



**YALITKAN PASPAS**  
— KAUÇUK ÜRÜNLERİ A.Ş. —



**TYPE 5B/6B**

**PROTECTIVE COVERALL**

- Made from Nonwoven + PE Film
- 55 - 60 gram / m<sup>2</sup>
- White Color



CAT III



Patojen Organizmalara Karşı Koruma  
Protection Against Pathogenic Organisms.  
EN 14126:2003 + AC:2004

**CE** 2163



Tehlikeli Kuru Partiküllere Karşı Koruma  
Type 5-B / Protection Against Hazardous  
EN 13982-1 :2004 + A1:2010



Hafif Pluskürtülen Partiküllere Karşı  
Koruma Type 6-B / Protection Against  
Hazardous Dry Particles Type 6-B.  
EN 13034:2005+A1:2009

ISO 9001:2015  
ISO 13485:2016  
OHSAS 18001:2007  
ISO 37001:2016  
ISO 26000-2010-SAB8000  
ISO 14001:2015



[www.yalitkanpaspas.com.tr](http://www.yalitkanpaspas.com.tr)

 [amsterdam\\_turkey](https://www.instagram.com/amsterdam_turkey)



# YALITKAN PASPAS

— KAUÇUK ÜRÜNLERİ A.Ş. —

Photo



Model

YLT - 01

General Features

- Disposable Coverall
- 55 - 60 GSM
- Full body protection
- CE Certified (EN 14126 : 2003+AC:2004)
- Certified by European Notify Body 2163 Universal
- Superior Coverall Fabric
- Aunotomic relax fit
- Designed to decrease Heat Stress



*One piece hooded design*



*Security tape*



*With zipper*



*Elastic waist*



*Elastic cuff*



*Flexible*



**AMSTERDAM**

**YALITKAN PASPAS**  
— KAUÇUK ÜRÜNLERİ A.Ş. —

**YOU**

**PROTECTIVE COVERALLS**

# AMSTERDAM



## TYPE 5-B/6-B CLASSIC COVERALL

### GÜVENLİK TALİMATI

Bütün koruyucu giysiler, kullanmadan önce, yırtık, delik, söküklük, kir gibi olumsuzluk yaratılacak defo ve arızalara karşı kontrol edilmelidir. Delolu ve kirlili ise kesinlikle giyilmemelidir.

### DIKKAT !

Pigele ile oynarken tehlikelidir, boğulmaya sebep olabilir, Lütfen çocuk ve bebeklerden uzak tutunuz.

### INSTRUCCIONES DE SEGURIDAD

Toda la ropa de protección debe controlarse antes de su uso contra defectos y fallos como las rasgaduras. Los agujeros, las rasgones y las suciedades. No deben usarse si tienen defectos y sucias.

### ATENCIÓN!

Es peligroso jugar con las bolsas puede causar asfixia. Por favor, mantenga alejado de los niños y bebés.

### BEZPEČNOSTNÍ POKYNY

Veškeré ochranné oděvy musí být před jejich použitím zkontrolovány, zda neobsahují negativní vadu nebo poškození, nejsou prasklé, děravé, roztrhané, roztrhané nebo špinavé. Poškozené oděvy by v žádném případě použity být neměly.

### UPOZORNĚNÍ !

Hráti si se sáčkem je nebezpečné, může dojít k udusení. Prosim uchovejte mimo dosah dětí.

### TURVAOHJEET

Kaikki suojavaatteet tulee tarkastaa aina ennen käyttöä mahdollisten reppien, reikien, painaumien, laur ym. haittojen varalta. Mahdollisten vaurioiden ja epäkohtaisuuksien varalta tulee aina tehdä tarkistus. Vihreillä tai ikkasia tuotetta ei missään nimessä tule käyttää.

### HUOMIO!

Pussin kanssa leikkiminen on vaarallista. Se voi aiheuttaa tukkimiskolonni. Pääkkä poissa lasten ja vauvojen ulottuvilta.

### BIZTONSÁGI ELŐIRÁSOK

Használatát elől minden viselőruhán meg kell vizsgálni azt, hogy van-e rálla szakadás, lyuk, varrási hibák, személyszerű vágás bármely olyan dolog ami problémát okozhatna.

### VEGYÁZATI!

A zacskóval játszani veszélyes, mert fufadást okozhat. Kérjük, tartsák távol a gyermekektől és a csecsemőktől!

### SAFETY INSTRUCTION

All protective clothing should be checked before use against defects and faults which may cause negatively such as tears, holes, rips and dirt. If it is detected and dirty, it should definitely not be worn.

### ATTENTION!

Playing with a bag is dangerous and can cause suffocation. Please keep away from children and infants.

### ISTRUZIONI DI SICUREZZA

Tutti gli indumenti protettivi devono essere controllati prima dell'utilizzo nei confronti di difetti e guasti che possono causare negativamente, quali difetti, fori, strappi e sporosità. Se è difettato e sporco, non dovrebbe essere indossato.

### ATTENZIONE!

Giocare con i sacchetti è pericoloso e può causare soffocamento. Si prega di tenere lontano da bambini e neonati.

### ПРАВИЛА БЕЗОПАСНОСТИ

Всю защитную одежду перед применением необходимо проверить на наличие дыр, разрывов швов, загромождений, а также нечистоты и повреждений. Покупенные, сползшие негатино оказаться на эффективности защиты. Ни в коем случае нельзя надевать поврежденную и загрязненную защитную одежду.

### ВНИМАНИЕ!

Нельзя играть с пакетами, возможны риск удушья. Пожалуйста, храните в местах, недоступных для младенцев и детей.

### ISTRUKCJA BEZPEČENSTWA

Wszystkie ubrania ochronne przed użyciem muszą być sprawdzone, czy nie są podarte, przecierane, rozprute, brudne albo nie posiadają innych nie pożądanych wad. Oczyszczony brudnych i wadami absolutnie nie należy zakładać.

### UWAGA!

Zabawa z torbką jest niebezpieczna, może spowodować uduszenie. Przechowywać z dala od dzieci i niemowląt.

### VARNOSTNA NAVODILA

Pred uporabo varnostnih oblačil, jih vedno preverite, da niso raztrgana, preluknjana, odrgana ali umazana, saj bi to negativno vplivalo na zaščito. Varnostnega oblačila ne smete uporabljati, če je umazano ali pokvarjeno.

### OPOROBLI!

Vredilo je graditi za dojenčkov in otrokov in lahko povzroči zadušitev, zato jo shranjajte stran od otrok.

### INSTRUCTION DE SÉCURITÉ

Tous les vêtements de protection doivent être vérifiés avant utilisation contre les défauts et les imperfections pouvant causer des négations tels que les déchirures, les trous, les déchirures et les saletés. Si elle est détériorée et sale, elle ne devrait certainement pas être portée.

### ATTENTION!

Jouer avec un sac est dangereux et peut provoquer un étouffement. Gardez-vous à l'écart des enfants et des nourrissons.

### INSTRUCÇÕES DE SEGURANÇA

Todas as roupas de proteção devem ser verificadas contra defeitos antes do uso, como rasgos e sujeira. Se é defeito e sujo, definitivamente não deve ser usado.

### ATENÇÃO!

Jogar com cobertura é perigoso e pode causar afogamento. Mantenha-se afastado de crianças e bebês.

### SIKKERHEDSINSTRUKTIONER

Før brug bør alle beskyttelsesklæder kontrolleres for revner, huller, ripede syninger, snavs som kan skabe negative virkninger samt for hull og mangler. Defekte og beskidte overtrækstrøkker bør ikke benyttes.

### ADVARSEL!

Det er farligt at lege med poserne, det kan forårsage kvælning. Opbevar venligst væk fra børn og spædbørn.

### SICHERUNGSANWEISUNG

Alle Schutzbekleidungen sollten vor Einsatz gegen Risse, Löcher, Laufmaschen und Probleme hervorrufoend sonstige Störungen zu kontrollieren. Gestörte und kontaminierte Anzüge nicht verwenden.

### ACHTUNG!

Das Spielen mit dem Beutel ist gefährlich und kann zum Erstickten führen. Bitte halten Sie den Beutel von Kindern und Kleinkindern fern.

### VEILIGHEIDVOORSCHRIFT

Alle beschermingsbedrungen moeten vooraf aanbreken gecontroleerd worden tegen gebreken en defecten zoals scheuren, gaten, open gesproongen stukken en vuil. Als deze gebrekkig of vuil is, moet bestel niet gebruikt worden.

### ATTENTE!

Het is gevaarlijk om met het zakje te spelen, het kan stikken veroorzaken. A.u.b. uit het zicht van kinderen en baby's houden.

### SÄKERHETSFÖRESKRIFTER

Före användning bör alla skyddskläder kontrolleras för sprickor, hål, slitning i sömmar, smuts och fet som kan orsaka negativa effekter. Defekta och smutsiga överkläder bör inte användas.

### VARNING!

Allt lek med ompackningen kan innebära fara och kan orsaka kvävning. Håll vifligen bort från barn och spädbarn.

### INSTRUCȚIUNI DE SIGURANȚĂ

Toată îmbrăcămintea de protecție trebuie să fie verificată înainte de utilizare pentru a controla în vederea depistării posibilelor imperfecțiuni și defecte cum ar fi rupături, găuri, deteriorări, mizerie. Nu trebuie utilizate sub nici o formă dacă prezintă imperfecțiuni și urme de mizerie.

### ATENȚIE!

Jocul cu punga este periculos, poate provoca asfixiere. Vă rugăm să păstrați în locuri inaccesibile copiilor și bebelușilor.

### توجيهات الأمان

يجب فحص كافة الملابس الواقية ضد الحوادث والحوادث قبل استخدامها للتأكد من خلوها من الشقوق والتمزقات والتلف في الخياطة، وكذلك من وجود بقع أو ملامح غير مرغوب فيها. لا ينبغي استخدام الملابس الواقية إذا كانت متسخة أو متضررة.

### تنبیه!

بازی با کیسه خطرناک است و می‌تواند منجر به خفگی شود. لطفاً این کیسه را از دسترس کودکان و نوزادان دور نگه دارید.



CAT III



Patogen Organizmalara Karşı Koruma  
Protection Against Pathogenic Organisms.  
EN 14126:2003 + AC:2004



Tehlikeli Kuru Partiküllere Karşı Koruma  
Type 5-B / Protection Against Hazardous  
EN 13992-1 :2004 + A1:2010



Hafif Püskürtülen Partiküllere Karşı  
Koruma Type 6-B / Protection Against  
Hazardous Dry Particles Type 6-B.  
EN 13034:2005+A 1 :2009

**Koruyucu Tulum LOT Kodu**  
Protective Overalls LOT Code



ISO 9001:2015  
ISO 13485:2016  
OHSAS 18001:2007  
ISO 37001:2016  
ISO 26000-2010-SAB000  
ISO 14001:2015



Do not Wash.  
Yıkamaz



Do not dry in dryer.  
Kurutma makinasında kurutulmaz



Do not clean with bleach.  
Kuru temizleme yapılmaz



Do not iron.  
Ütülenmez



Do not use Bleach.  
Çamaşır suyu kullanılmaz



Do not use twice.  
2 kez kullanılmaz  
Tek kullanılır



Keep Away From Fire.  
Ateşten Uzak Tutunuz

MEKANİK DAYANIM SINIFLARI / MECHANICAL TRENGTH CLASSES	
Aşınma Direnci / Abrasion Resistance	Sınıf / Class 6
Yırtılma Direnci / Tear Resistance	Sınıf / Class 2
Çekme Mukavemeti / Tensile Strength	Sınıf / Class 2
Delinme Direnci / Puncture Resistance	Sınıf / Class 1
Dikiş Mukavemeti / Seam Strength	Sınıf / Class 2

Ürün giymeye ve ürün çıkarmaya talimatı gösterileceği gibidir.

The instructions for dressing the product and removing the product are as in the picture.

## DISPOSABLE PROTECTIVE COVERALL



Size	Person's Length (cm) A	Person's Chest (cm) B
S	186	60
M	189	62
L	192	64
XL	198	66
2XL	204	70
3XL	210	74
4XL	216	78
Tolerance $\pm 3$		



PACKAGE SIZE: 60x40x40 cm

1 BOX: 50 Pcs

1 PALLET: 1000 Pcs / 20 Box

1 TRUCK: 33 Pallets

## EU TYPE EXAMINATION CERTIFICATE

Certificate No: [REDACTED]

### YALITKAN PASPAS KAUÇUK ÜRÜNLERİ A.Ş.

Oruçreis Mah. Tekstilkent Cad. Tekstilkent Gd1 Blok No:148 Esenler İstanbul TURKEY

It is certified that the manufacturer's technical file (Dated 19.11.2020) and the PPE product, detailed below, have been assessed and found to meet the applicable Essential Health and Safety Requirements in Annex II of Regulation (EU) 2016/425 based on the evaluation on technical documentation and relevant test reports.

#### Identification of the Personal Protective Equipment

Brand Name: AMSTERDAM, Model: YLT01

Protective coverall manufactured from white laminated polypropylene non-woven fabric with hood, inside overlock seams, elastic cuff, ankle and waist, zipper and zipper flap. The coverall is available in 6 nominal sizes.

#### The following harmonised standards have been applied:


EN ISO 13688:2013, (General requirements for protective clothing)  
EN ISO 13982-1:2004/A1:2010, (Chemical protective clothing providing protection to the full body against airborne solid particulates) Type 5, limited wear life clothing,  
EN 13034:2005+A1:2009, (Chemical protective clothing offering limited protective performance against liquid chemicals) Type 6, limited wear life clothing,  
EN 14126:2003/AC:2004, (Protective clothing against infective agents) for Type 5-B, 6-B.

Here by the manufacturer is allowed to use notified body number (2163) and can fix CE mark, as shown below, on the Category III product models given above, with the below requirements;

- Issuing an appropriate EU Declaration of Conformity according to **Personal Protective Equipment Regulation (EU) 2016/425 Annex 9.**
- Ongoing successful performance in fulfilment of the requirements set out in Personal Protective Equipment Regulation (EU) 2016/425 and harmonised standards, ensured by assessments based on Annex 7 (Module C2) or Annex 8 (Module D) of the regulation

This certificate is initially issued on 09/12/2020 and will be valid for 5 years from the issue date.



  
Suat KACMAZ  
UNIVERSAL CERTIFICATION  
Director

## EU DECLARATION OF CONFORMITY

### MANUFACTURER

YALITKAN PASPAS KAUÇUK ÜRÜNLERİ A.Ş.

Oruçreis Mah. Tekstilkent Cad. Tekstilkent Gd1 Blok No:148 Esenler-İstanbul/TURKEY

### PRODUCT DESCRIPTION

Brand Name: AMSTERDAM, Model: YLT01

Protective coverall manufactured from white laminated polypropylene non-woven fabric with hood, inside overlock seams, elastic cuff, ankle and waist, zipper and zipper flap. The coverall is available in 6 nominal sizes.

Type 5 – Providing Protection to the Full Body against Airborne Solid Particulates

Type 6 – Offering Limited Protective Performance against Liquid Chemicals

Type 5-B, Type 6-B, Protective clothing against infective agents

The Manufacturer declares on his sole responsibility that the product above is, under conditions of normal use and conditions defined by the Manufacturer, safe and meets all the necessary legal conditions and requirements. The product is a personal protective equipment that is intended for single use and solely in accordance with the Manufacturer's instructions.

#### The Conformity is assessed with the following mechanism:


- Complies with EU 2016/425 Personal Protective Equipment Regulation establishing technical requirements for Category III products,
- Complies with Technical harmonised standards in accordance the Essential Health and Safety Requirement referenced to EU 2016/425 PPE Regulation, EN ISO 13688:2013, EN 14126:2003/AC:2004, EN ISO 13982-1:2004/A1:2010, EN 13034:2005+A1:2009
  - All required tests referred in above standards are conducted,
  - Complies with other relevant harmonized legislation and community standards
- For the assessment of conformity the EU Type Examination certificate is issued, after all technical evaluations for conformity to the regulation and harmonised standards conducted under supervision of,
- UNIVERSAL CERTIFICATION, SURVEILLANCE SERVICES and TRADE Co, Notified Body number 2163

#### MARKING, LABELLING

Marking, labelling and user information are prepared in accordance with EU 2016/425 Personal Protective Equipment Regulation and EN 14126. The information is supplied with the product considering EN ISO 15223-1:2006 and EN 1041:2008+A1:2013

#### MEASURES TO ENSURE CONFORMITY

The Manufacturer declares that he has taken all necessary measures to ensure the conformity of products placed on the market with technical documentation and technical requirements for his type of product.

 **YALITKAN PASPAS**  
KAUÇUK ÜRÜNLERİ A.Ş.  
Oruçreis Mah. Tekstilkent Cad. Tekstilkent Gd1  
No:148 AE Daire No: 230 Esenler / İSTANBUL  
Atölyeleri V.D.: 93340926/51 - Sicil No: 223853-5  
Mersis No: 0933092605100001  
Engin Özavcı

General Manager

09/12/2020



**TECHNICAL EVALUATION REPORT**

**REPORT DATE / NO:** 09.12.2020 / 2163-KKD-1761

**Applicant:** YALITKAN PASPAS KAUCUK ÜRÜNLERİ A.Ş.

**Address:** Oruçreis Mah. Tekstilkent Cad. Tekstilkent Gd1 Blok No:148 Esenler İstanbul TURKEY

**Introduction**

This report is prepared based on the evaluations on the technical file of the manufacturer dated 19 November, 2020 Version 0, and the test reports obtained from the laboratories for the analysis referenced by the applied harmonised standards for the personal protective equipment identified below. A list to the test reports is given below which are referenced within this report. The samples for evaluation are provided by the manufacturer for type examination and samples are delivered to the laboratories under UNIVERSAL supervision. The test results and all evaluations within this report belongs to the samples provided.

This report is prepared for the PPE with the guidance of the harmonised standards which are claimed to be applied by the manufacturer and the evaluation is conducted for the verification of fulfilment of Essential Health and Safety Requirements of PPE regulation, those applies for the product.

**PPE Identification:** Protective coverall manufactured from white laminated polypropylene non-woven fabric with hood, overlock seams, elastic cuff, ankle and waist, zipper and zipper flap. The coverall is available in 6 nominal sizes.

**Component and Materials:**

**Fabric:** 57 gr Non Woven Fabric (30gr Non Woven + 25gr PE Film + 2gr Adhesive)

**Zipper:** Polyester Woven Zipper

**Coverall Type:** Type 5-B / Type 6-B

**Brand Name:** AMSTERDAM

**Model:** YLT01

**Sizes Available:** S - M - L - XL - 2XL - 3XL

**Applied Harmonised Standards**

EN ISO 13688:2013, (General requirements for protective clothing)

EN ISO 13982-1:2004/A1:2010, (Chemical protective clothing providing protection to the full body against airborne solid particulates) Type 5, limited wear life clothing,

EN 13034:2005+A1:2009, (Chemical protective clothing offering limited protective performance against liquid chemicals) Type 6, limited wear life clothing,

EN 14126:2003/AC:2004, (Protective clothing against infective agents) for Type 5-B, 6-B limited life, full body protection

This report is prepared on the basis of applicable Essential Health and Safety Requirements with the references annexed to each applied harmonised standard given above.

**TEST REPORT INFORMATION**

Report #	Laboratory Name	Report Date and Number	Competency Reference
1	Ekoteks Laboratuvar ve Gözetim Hizmetleri A.Ş.	Dated 12.11.2020 Number: 20041658	Holds TURKAK Accreditation with No: AB-0583-T
2	GCNTR - Global Technology Laboratory	Dated 12.11.2020 # GTL-TLM-0078A/20	Holds TURKAK Accreditation with No: AB-1252-T
3	GCNTR - Global Technology Laboratory	Dated 12.11.2020 # GTL-TLM-0078/20	Holds TURKAK Accreditation with No: AB-1252-T
4	Çevre Endüstriyel Analiz Laboratuvarı	Dated 17.11.2020 Number: 2028323E	Holds TURKAK Accreditation with No: AB-0363-T

The laboratories are contracted bodies with UNIVERSAL and the technical competence of the laboratories is also under supervision / assessment of UNIVERSAL based on the provisions of EN ISO/IEC 17065 Requirements for bodies certifying products, processes and services standard.



**ESSENTIAL HEALTH and SAFETY REQUIREMENTS GIVEN IN EUROPEAN UNION REGULATION EU 2016/425 CORRESPONDING to Annex ZA of EN ISO 13688:2013 STANDARD**

**1. GENERAL REQUIREMENTS APPLICABLE TO ALL PPE**

**1.2. Innocuousness of PPE**

**1.2.1. Absence of inherent risks and other nuisance factors**

PPE must be designed and manufactured so as not to create risks or other nuisance factors under foreseeable conditions of use.

**1.2.1.1. Suitable constituent materials**

The materials of which the PPE is made, including any of their possible decomposition products, must not adversely affect the health or safety of users

**1.2.1.2. Satisfactory surface condition of all PPE parts in contact with the user**

Any part of the PPE that is in contact or is liable to come into contact with the user when the PPE is worn must be free of rough surfaces, sharp edges, sharp points and the like which could cause excessive irritation or injuries.

**1.4. Manufacturer's instructions and information**

In addition to the name and address of the manufacturer, the instructions that must be supplied with the PPE must contain all relevant information on:

- instructions for storage, use, cleaning, maintenance, servicing and disinfection. Cleaning, maintenance or disinfectant products recommended by manufacturers must have no adverse effect on the PPE or the user when applied in accordance with the relevant instructions;
- performance as recorded during relevant technical tests to check the levels or classes of protection provided by the PPE;
- where applicable, accessories that may be used with the PPE and the characteristics of appropriate spare parts;
- where applicable, the classes of protection appropriate to different levels of risk and the corresponding limits of use;
- where applicable, the month and year or period of obsolescence of the PPE or of certain of its components;
- where applicable, the type of packaging suitable for transport;
- the significance of any markings (see point 2.12);
- the risk against which the PPE is designed to protect;
- the reference to this Regulation and, where applicable, the references to other Union harmonisation legislation;
- the name, address and identification number of the notified body or bodies involved in the conformity assessment of the PPE;
- references to the relevant harmonised standard(s) used, including the date of the standard(s), or references to the other technical specifications used;
- the internet address where the EU declaration of conformity can be accessed.

The information referred to in points (i), (j), (k) and (l) need not be contained in the instructions supplied by the manufacturer if the EU declaration of conformity accompanies the PPE.

**2. ADDITIONAL REQUIREMENTS COMMON TO SEVERAL TYPES OF PPE**

**2.12. PPE bearing one or more identification markings or indicators directly or indirectly relating to health and safety**


Where PPE bears one or more identification markings or indicators directly or indirectly relating to health and safety, those identification markings or indicators must, if possible, take the form of harmonised pictograms or ideograms. They must be perfectly visible and legible and remain so throughout the foreseeable useful life of the PPE. In addition, those markings must be complete, precise and comprehensible so as to prevent any misinterpretation. In particular, where such markings include words or sentences, the latter must be written in a language easily understood by consumers and other end-users, as determined by the Member State where the PPE is made available on the market.


Where PPE is too small to allow all or part of the necessary marking to be affixed, the relevant information must be mentioned on the packaging and in the manufacturer's instructions.



Technical Assessment of EN ISO 13688: 2013 Standard and other Standards it refers to, Clauses Corresponding to the Essential Health and Safety Requirements given above

**EN ISO 13688 Standard Requirements Evaluation**
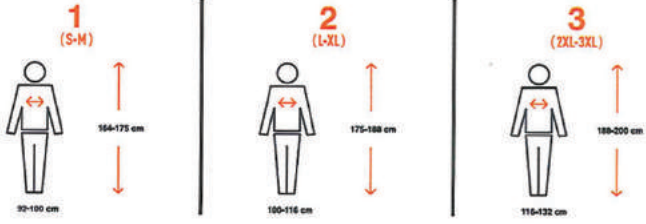
<i>Article 4.2</i>	<p>EHSR Ref 1.2.1.1;          The manufacturer declares in his technical file that the materials used in the manufacturing process of this specific PPE do not adversely affect the health or hygiene of the user. The manufacturer claims that the materials do not, in the foreseeable conditions of normal use, release substances generally known to be toxic, carcinogenic, mutagenic, allergenic, toxic to reproduction or otherwise harmful.          Ref: Technical File Article 3</p>
<i>Article 4.4</i>	<p>EHSR Ref 1.2.1.2;          The comfort of the PPE was subject to visual inspection by our experts for rough, sharp or hard surfaces that irritate or injure the user and found to be appropriate for use. In addition such properties of the PPE was subject to evaluation during the practical exercise testing as defined in the EN ISO 17491-4 testing standard and the PPE is reported as to be comfortable enough to allow the wearer to complete the exercises.          Ref: Test Reports.</p>
<i>Article 5.3</i>	<p>EHSR Ref 1.2.1;          The samples received from the manufacturer are claimed to be single use. No further evaluation is conducted on the dimensional change due to cleaning.          Ref: Technical File Article 6.</p>
<i>Article 6</i>	<p>EHSR Ref 2.12;          The coverall is available in 6 nominal sizes. The nominal sizes are defined in the technical file of the manufacturer. The given dimensions in chest or bust girth and height are found in the limits defined in Annex D of the standard.</p> <div style="text-align: center;">  </div> <p>Ref: Technical File Article 10.</p>
<i>Article 7</i>	<p>EHSR Ref 2.12;          Each piece of coverall have marking with the following information;</p> <ul style="list-style-type: none"> <li>Name / trademark of the manufacturer, type of product</li> <li>Size of the coverall</li> <li>Applied product standards (Type defining product standards)</li> <li>Applied protection pictograms with standard references</li> </ul> <p>The markings on the coverall / label are found to be easily visible and enough big to read. The marking rules are explained in the marking section of the technical file. For further clarifications for the marking requirements of applied product standards are available in the relevant standard section of this report.</p>



**EN ISO 13688 Standard Requirements Evaluation**

<i>Article 8</i>	<p>EHSR Ref 1.4;          The information supplied by the manufacturer is defined in the relevant section of the technical file. This information includes explanation required by all applied product standard requirements. The defined user information text in the technical file includes the following data;</p> <ul style="list-style-type: none"> <li>Name / trademark of the manufacturer, its address,</li> <li>Applied standards and relevant classification, marking, size information</li> <li>Pictograms and explanations</li> <li>Coverall constituent materials used</li> <li>Instructions for use, controls before use, how to wear / unwear, limitations, instructions for storage conditions, complementary PPEs, re-usability, instructions for disposal</li> </ul> <p>The above user information text is available in Turkish.</p>
------------------	---



## 1. GENERAL REQUIREMENTS APPLICABLE TO ALL PPE

### 1.1. Design principles

#### 1.1.1. Ergonomics

PPE must be designed and manufactured so that, in the foreseeable conditions of use for which it is intended, the user can perform the risk-related activity normally whilst enjoying appropriate protection of the highest level possible.

#### 1.1.2. Levels and classes of protection

##### 1.1.2.1 Optimum level of protection

The optimum level of protection to be taken into account in the design is that beyond which the constraints imposed by the wearing of the PPE would prevent its effective use during the period of exposure to the risk or the normal performance of the activity.

#### 1.2. Innocuousness of PPE

##### 1.2.1. Absence of inherent risks and other nuisance factors

PPE must be designed and manufactured so as not to create risks or other nuisance factors under foreseeable conditions of use.

##### 1.2.1.1. Suitable constituent materials

The materials of which the PPE is made, including any of their possible decomposition products, must not adversely affect the health or safety of users

##### 1.2.1.2. Satisfactory surface condition of all PPE parts in contact with the user

Any part of the PPE that is in contact or is liable to come into contact with the user when the PPE is worn must be free of rough surfaces, sharp edges, sharp points and the like which could cause excessive irritation or injuries.

##### 1.2.1.3. Maximum permissible user impediment

Any impediment caused by PPE to the actions to be carried out, the postures to be adopted and sensory perceptions shall be minimised. Furthermore, use of the PPE must not engender actions which might endanger the user.

#### 1.3. Comfort and effectiveness

##### 1.3.1. Adaptation of PPE to user morphology

PPE must be designed and manufactured in such a way as to facilitate its correct positioning on the user and to remain in place for the foreseeable period of use, bearing in mind ambient factors, the actions to be carried out and the postures to be adopted. For this purpose, it must be possible to adapt the PPE to fit the morphology of the user by all appropriate means, such as adequate adjustment and attachment systems or the provision of an adequate range of sizes.

##### 1.3.2. Lightness and strength

PPE must be as light as possible without prejudicing its strength and effectiveness. PPE must satisfy the specific additional requirements in order to provide adequate protection against the risks for which it is intended and PPE must be capable of withstanding environmental factors in the foreseeable conditions of use.


##### 1.3.3. Compatibility of different types of PPE intended for simultaneous use

If the same manufacturer places on the market several PPE models of different types in order to ensure the simultaneous protection of adjacent parts of the body, they must be compatible.

#### 1.4. Manufacturer's instructions and information

In addition to the name and address of the manufacturer, the instructions that must be supplied with the PPE must contain all relevant information on:

- instructions for storage, use, cleaning, maintenance, servicing and disinfection. Cleaning, maintenance or disinfectant products recommended by manufacturers must have no adverse effect on the PPE or the user when applied in accordance with the relevant instructions;
- performance as recorded during relevant technical tests to check the levels or classes of protection provided by the PPE;



- where applicable, accessories that may be used with the PPE and the characteristics of appropriate spare parts;
- where applicable, the classes of protection appropriate to different levels of risk and the corresponding limits of use;
- where applicable, the month and year or period of obsolescence of the PPE or of certain of its components;
- where applicable, the type of packaging suitable for transport;
- the significance of any markings (see point 2.12);
- the risk against which the PPE is designed to protect;
- the reference to this Regulation and, where applicable, the references to other Union harmonisation legislation;
- the name, address and identification number of the notified body or bodies involved in the conformity assessment of the PPE;
- references to the relevant harmonised standard(s) used, including the date of the standard(s), or references to the other technical specifications used;
- the internet address where the EU declaration of conformity can be accessed.

The information referred to in points (i), (j), (k) and (l) need not be contained in the instructions supplied by the manufacturer if the EU declaration of conformity accompanies the PPE.

## 2. ADDITIONAL REQUIREMENTS COMMON TO SEVERAL TYPES OF PPE

### 2.12. PPE bearing one or more identification markings or indicators directly or indirectly relating to health and safety

Where PPE bears one or more identification markings or indicators directly or indirectly relating to health and safety, those identification markings or indicators must, if possible, take the form of harmonised pictograms or ideograms. They must be perfectly visible and legible and remain so throughout the foreseeable useful life of the PPE. In addition, those markings must be complete, precise and comprehensible so as to prevent any misinterpretation. In particular, where such markings include words or sentences, the latter must be written in a language easily understood by consumers and other end-users, as determined by the Member State where the PPE is made available on the market.

Where PPE is too small to allow all or part of the necessary marking to be affixed, the relevant information must be mentioned on the packaging and in the manufacturer's instructions.

## 3. ADDITIONAL REQUIREMENTS SPECIFIC TO PARTICULAR RISKS

### 3.10. Protection against substances and mixtures which are hazardous to health and against harmful biological agents

#### 3.10.2. Protection against cutaneous and ocular contact

PPE intended to prevent the surface contact of all or part of the body with substances and mixtures which are hazardous to health or with harmful biological agents must be capable of preventing the penetration or permeation of such substances and mixtures and agents through the protective integument under the foreseeable conditions of use for which the PPE is intended.

To this end, the constituent materials and other components of those types of PPE must be chosen or designed and incorporated so as to ensure, as far as possible, complete leak-tightness, which will allow where necessary prolonged daily use or, failing this, limited leak-tightness necessitating a restriction of the period of wear.

Where, by virtue of their nature and the foreseeable conditions of their use, certain substances and mixtures which are hazardous to health or harmful biological agents possess high penetrative power which limits the duration of the protection provided by the PPE in question, the latter must be subjected to standard tests with a view to their classification on the basis of their performance. PPE which is considered to be in conformity with the test specifications must bear a marking indicating, in particular, the names or, in the absence of the names, the codes of the substances used in the tests and the corresponding standard period of protection. The manufacturer's instructions must also contain, in particular, an explanation of the codes (if necessary), a detailed description of the standard tests and all appropriate information for the determination of the maximum permissible period of wear under the different foreseeable conditions of use.





Technical Assessment of EN ISO 13982-1:2004 + A1:2010 Standard and other Standards it refers to, Clauses Corresponding to the Essential Health and Safety Requirements given above

**EN ISO 13982-1:2004 + A1:2010 Standard Requirements Evaluation**

EHSR Ref 1.2.1, 1.3.2;

The overall material performance are tested according to EN 14325:2018 standard for the following properties, since the overall is claimed to be for single use no cleaning cycle is applied;

Property of Material EN 14325:2018	Result Classification		Requirement of EN ISO 13982-1	Evaluation
4.4 Abrasion Resistance	No Abrasion @2000 revs	Class 6	Class 1 or above	Success
4.5 Flex cracking resistance	> 5,000 Cycles	Class 3	Class 1 or above	Success
4.7 Trapezoidal tear resistance	Width 54.63 N Length 27.81 N	Class 2	Class 1 or above	Success
4.10 Puncture Resistance	6.5 N	Class 1	Class 1 or above	Success

The above results are derived from the test report, in the reference below. In the evaluation of the test report it was stated that all the tests are conducted with the completion of conditioning requirements as (20 ± 2) C° and (65 ± 5) % relative humidity for 24 hours.

The manufacturer do not claim a performance for the resistance to ignition or flammability of the product, in the user information sheet it is explained that the coveralls must be kept away of fire. Other requirements referred for skin compatibility, no irritation or adverse effects are evaluated in EN ISO 13688 section of this report.

Ref: Laboratory Test Report 1, Technical File

EHSR Ref 1.3.2, 3.10.2;

The affects of seams to the performance of the coverall in penetration of solid particles through stitch holes are evaluated in the whole suit test and evaluated in Article 4.3 of this section.

The seam strength is evaluated based on the test report as shown below;

Property of Material EN 14325:2018	Result Classification		Requirement of EN ISO 13982-1	Evaluation
5.5 Seam Strength	Refer to the strength values for seams at different parts of coverall. The lowest Class is given among all kinds of seams	Class 2	Class 1 or above	Success

Ref: Laboratory Test Report 1

EHSR Ref 1.1.1, 1.1.2.1, 1.2.1.2, 1.2.1.3, 1.3.1, 1.3.3, 3.10.2;

The requirements of the coverall with respect to health and safety, ageing and sizing are evaluated in EN ISO 13688 section of this report.

The coverall under evaluation is a one piece full body clothing, without a visor and foot protection. The necessary additional PPEs must be worn by the wearer for the intended use. The freedom of movements of the wearer is tested as a part of the Total Inward Leakage test and found to be appropriate.

According to the test results reported;

- The subjects were able to complete the exercises described comfortably. The inspection on the tested samples states that there was no damage, tears or rips in fabrics, seams and connection points to the additionally worn PPEs like gloves, boots etc.

**EN ISO 13982-1:2004 + A1:2010 Standard Requirements Evaluation**

- The results of percentages of inward leakage values reported claims that all 90 measurements are smaller and equal to 30. Which means 90 of the total leakage measurement among all exercises for all positions and all samples are smaller than 30%.
- All 10 of the average total inward leakage per tested suit are smaller or equal to 15%.

The above results indicates that the tested coveralls complies with the total inward leakage of aerosols of solid particles requirement of this standard. Which is based on a test report conducted according to EN ISO 13982-2:2005

Ref: Laboratory Test Report 2

EHSR Ref 2.12;

Each piece of coverall have marking with the following information on the single PPE package / PPE itself;

- Name / trademark of the manufacturer, type and model of PPE
- Size of the coverall
- Applied product standards (EN ISO 13982-1+A1:2010)
- Pictograms for protection against chemicals, invitation to read manufacturer's instructions
- Shelf life and date of manufacturing

The above mentioned marking requirements are stated in the technical file of the manufacturer. The evaluated samples did not have all these marking and information on the PPE. The manufacturer shall follow the instructions in the technical file in case of serial manufacturing of the PPE and verify before putting the PPE on the market. The PPE coverall is for single use, the markings for re-use cleaning or disinfection is discarded.

Ref: Technical File PPE Marking section.

EHSR Ref 1.4;

The information supplied by the manufacturer is defined in the relevant section of the technical file. This information includes explanation required by all applied product standard requirements. The defined user information text in the technical file includes the following data;

- Name / trademark of the manufacturer, its address, or the authorised representative for EU community
- Type of protection against chemicals (Type-5). The information also includes a reminder for wearing necessary additional PPE in order to achieve a full body protection (i.e boots, gloves, mask and visor / face shield).
- Size of the coverall
- The statement that the coverall provides a total inward leakage  $L_{jmm,82/90} \leq 30\%$  and  $L_{s,8/10} \leq 15\%$
- Material test performance classifications (Based on EN 14325:2018 classification)
- Pictogram and information that the PPE is non-reusable also the shelf life is mentioned
- Instructions for use, controls before use, how to wear / unwear, limitations, instructions for storage conditions, complementary, instructions for disposal

The above user information text is available in Turkish.

Ref Technical File, User Information Sheet

Article 6

## 1. GENERAL REQUIREMENTS APPLICABLE TO ALL PPE

### 1.1. Design principles

#### 1.1.1. Ergonomics

PPE must be designed and manufactured so that, in the foreseeable conditions of use for which it is intended, the user can perform the risk-related activity normally whilst enjoying appropriate protection of the highest level possible.

#### 1.2. Innocuousness of PPE

##### 1.2.1. Absence of inherent risks and other nuisance factors

PPE must be designed and manufactured so as not to create risks or other nuisance factors under foreseeable conditions of use.

##### 1.2.1.1. Suitable constituent materials

The materials of which the PPE is made, including any of their possible decomposition products, must not adversely affect the health or safety of users

##### 1.2.1.3. Maximum permissible user impediment

Any impediment caused by PPE to the actions to be carried out, the postures to be adopted and sensory perceptions shall be minimised. Furthermore, use of the PPE must not engender actions which might endanger the user.

### 1.3. Comfort and effectiveness

#### 1.3.2. Lightness and strength

PPE must be as light as possible without prejudicing its strength and effectiveness. PPE must satisfy the specific additional requirements in order to provide adequate protection against the risks for which it is intended and PPE must be capable of withstanding environmental factors in the foreseeable conditions of use.


#### 1.3.3. Compatibility of different types of PPE intended for simultaneous use

If the same manufacturer places on the market several PPE models of different types in order to ensure the simultaneous protection of adjacent parts of the body, they must be compatible.

### 1.4. Manufacturer's instructions and information

In addition to the name and address of the manufacturer, the instructions that must be supplied with the PPE must contain all relevant information on:

- instructions for storage, use, cleaning, maintenance, servicing and disinfection. Cleaning, maintenance or disinfectant products recommended by manufacturers must have no adverse effect on the PPE or the user when applied in accordance with the relevant instructions;
- performance as recorded during relevant technical tests to check the levels or classes of protection provided by the PPE;
- where applicable, accessories that may be used with the PPE and the characteristics of appropriate spare parts;
- where applicable, the classes of protection appropriate to different levels of risk and the corresponding limits of use;
- where applicable, the month and year or period of obsolescence of the PPE or of certain of its components;
- where applicable, the type of packaging suitable for transport;
- the significance of any markings (see point 2.12);
- the risk against which the PPE is designed to protect;
- the reference to this Regulation and, where applicable, the references to other Union harmonisation legislation;
- the name, address and identification number of the notified body or bodies involved in the conformity assessment of the PPE;
- references to the relevant harmonised standard(s) used, including the date of the standard(s), or references to the other technical specifications used;
- the internet address where the EU declaration of conformity can be accessed.



The information referred to in points (i), (j), (k) and (l) need not be contained in the instructions supplied by the manufacturer if the EU declaration of conformity accompanies the PPE.

## 2. ADDITIONAL REQUIREMENTS COMMON TO SEVERAL TYPES OF PPE

### 2.4. PPE subject to ageing

If it is known that the design performance of new PPE may be significantly affected by ageing, the month and year of manufacture and/or, if possible, the month and year of obsolescence must be indelibly and unambiguously marked on each item of PPE placed on the market and on its packaging.

If the manufacturer is unable to give an undertaking with regard to the useful life of the PPE, his instructions must provide all the information necessary to enable the purchaser or user to establish a reasonable obsolescence month and year, taking into account the quality level of the model and the effective conditions of storage, use, cleaning, servicing and maintenance.

Where appreciable and rapid deterioration in PPE performance is likely to be caused by ageing resulting from the periodic use of a cleaning process recommended by the manufacturer, the latter must, if possible, affix a marking to each item of PPE placed on the market indicating the maximum number of cleaning operations that may be carried out before the equipment needs to be inspected or discarded. Where such a marking is not affixed, the manufacturer must give that information in his instructions.

### 2.12. PPE bearing one or more identification markings or indicators directly or indirectly relating to health and safety

Where PPE bears one or more identification markings or indicators directly or indirectly relating to health and safety, those identification markings or indicators must, if possible, take the form of harmonised pictograms or ideograms. They must be perfectly visible and legible and remain so throughout the foreseeable useful life of the PPE. In addition, those markings must be complete, precise and comprehensible so as to prevent any misinterpretation. In particular, where such markings include words or sentences, the latter must be written in a language easily understood by consumers and other end-users, as determined by the Member State where the PPE is made available on the market.

Where PPE is too small to allow all or part of the necessary marking to be affixed, the relevant information must be mentioned on the packaging and in the manufacturer's instructions.

## 3. ADDITIONAL REQUIREMENTS SPECIFIC TO PARTICULAR RISKS

### 3.10. Protection against substances and mixtures which are hazardous to health and against harmful biological agents

#### 3.10.2. Protection against cutaneous and ocular contact

PPE intended to prevent the surface contact of all or part of the body with substances and mixtures which are hazardous to health or with harmful biological agents must be capable of preventing the penetration or permeation of such substances and mixtures and agents through the protective integument under the foreseeable conditions of use for which the PPE is intended.

To this end, the constituent materials and other components of those types of PPE must be chosen or designed and incorporated so as to ensure, as far as possible, complete leak-tightness, which will allow where necessary prolonged daily use or, failing this, limited leak-tightness necessitating a restriction of the period of wear.

Where, by virtue of their nature and the foreseeable conditions of their use, certain substances and mixtures which are hazardous to health or harmful biological agents possess high penetrative power which limits the duration of the protection provided by the PPE in question, the latter must be subjected to standard tests with a view to their classification on the basis of their performance. PPE which is considered to be in conformity with the test specifications must bear a marking indicating, in particular, the names or, in the absence of the names, the codes of the substances used in the tests and the corresponding standard period of protection. The manufacturer's instructions must also contain, in particular, an explanation of the codes (if necessary), a detailed description of the standard tests and all appropriate information for the determination of the maximum permissible period of wear under the different foreseeable conditions of use.



Technical Assessment of EN ISO 13034:2005 + A1:2009 Standard and other Standards it refers to, Clauses Corresponding to the Essential Health and Safety Requirements given above

**EN ISO 13034:2005 + A1:2009 Standard Requirements Evaluation**

EHSR Ref 1.2.1, 1.2.1.1, 1.3.2, 3.10.2;

The coverall material performance are tested according to EN 14325:2018 standard for the following properties, since the coverall is claimed to be for single use no cleaning cycle is applied;

Property of Material EN 14325:2018	Result Classification	Requirement of EN ISO 13034	Evaluation	
4.4 Abrasion Resistance	No Abrasion @2000 revs	Class 6	Class 1 or above	Success
4.7 Trapezoidal tear resistance	Width 54.63 N Length 27.81 N	Class 2	Class 1 or above	Success
4.9 Tensile Strength	W 115.7 N L 46.5 N	Class 1	Class 1 or above	Success
4.10 Puncture Resistance	6.5 N	Class 1	Class 1 or above	Success
4.12 Liquid repellency	Sulfuric Acid (H <sub>2</sub> SO <sub>4</sub> ) (Concentration 30%) I <sub>R</sub> is 96.33 % Sodium Hydroxide (NaOH) (Concentration 10%) I <sub>R</sub> is 96.16 % o-Xylene (Undiluted) I <sub>R</sub> is 94.01 %	Class 3	Class 3 at least for 1 chemical	Success
4.10 Resistance to penetration by liquids	Sulfuric Acid (H <sub>2</sub> SO <sub>4</sub> ) (Concentration 30%) I <sub>P</sub> is 0 % Sodium Hydroxide (NaOH) (Concentration 10%) I <sub>P</sub> is 0 % o-Xylene (Undiluted) I <sub>P</sub> is 0 %	Class 3	Class 2 at least for 1 chemical	Success

Article 4.1

The above results are derived from the test report in the reference below. In the evaluation of the test report it was stated that all the tests are conducted with the completion of conditioning requirements as (20 ± 2) C° and (65 ± 5) % relative humidity for 24 hours.

The manufacturer do not claim a performance for the resistance to ignition or flammability of the product, in the user information sheet it is explained that the coveralls must be kept away of fire.

Other requirements referred for skin compatibility, no irritation or adverse effects are evaluated in EN ISO 13688 section of this report.

Ref: Laboratory Test Report 1, Technical File

EHSR Ref 1.3.2, 3.10.2;

The affects of seams to the performance of the coverall in penetration of liquid through stitch holes or through other components of a seam are evaluated in the whole suit mist test and evaluated in Article 5.2 of this section.

The seam strength is evaluated based on the test report as shown below;

Property of Material EN 14325:2018	Result Classification	Requirement of EN ISO 13034	Evaluation	
5.5 Seam Strength	Refer to the strength values for seams at different parts of coverall. The lowest Class is given among all kinds of seams	Class 2	Class 1 or above	Success

Ref: Laboratory Test Report 1

**EN ISO 13034:2005 + A1:2009 Standard Requirements Evaluation**

EHSR Ref 1.2.1.3, 2.4, 3.10.2;

The requirements of the coverall with respect to health and safety, ageing and sizing are evaluated in EN ISO 13688 section of this report.

The coverall under evaluation is a one piece full body clothing, without a visor and foot protection. The necessary additional PPEs must be worn by the wearer for the intended use. The freedom of movements of the wearer is tested as a part of the light spray (mist) test (Seven Movements) and found to be appropriate.

The test report claims the light spray test that it is conducted according to Method A of EN ISO 17491-4 which corresponds the test setup defined in Clause 5.2 of this standard.

According to the test results reported;

Article 5.1,5.2

- The subjects were able to complete the exercises (seven movements) described comfortably. The inspection on the tested samples states that there was no damage, tears or rips in fabrics, seams and connection points to the additionally worn PPEs like gloves, boots etc.
- The calibrated stain area is calculated for the undergarment is 4.56 cm<sup>2</sup>. The laboratory reports that for the 3 samples tested the total stain are of undergarments are smaller then three times the calibrated stain area, values are (0 cm<sup>2</sup>, 0 cm<sup>2</sup>, 3,8 cm<sup>2</sup>). For more details please refer to the test report.

The above results indicates that the tested coveralls complies with the resistance to penetration by liquids in the form of a light spray (mist) test requirement of this standard. Which is based on a test report conducted according to EN ISO 17491-4:2008+A1:2016.

Ref: Laboratory Test Report 3

EHSR Ref 2.12;

Each piece of coverall have marking with the following information on the single PPE package / PPE itself;

Article 6

- Name / trademark of the manufacturer, type and model of PPE
- Size of the coverall
- Applied product standards (EN ISO 13034:2005+A1:2009)
- Pictograms for protection against chemicals, invitation to read manufacturer's instructions
- Shelf life and date of manufacturing

The above mentioned marking requirements are stated in the technical file of the manufacturer. The evaluated samples did not have all these marking and information on the PPE. The manufacturer shall follow the instructions in the technical file in case of serial manufacturing of the PPE and verify before putting the PPE on the market. The PPE coverall is for single use, the markings for re-use cleaning or disinfection is discarded.

Ref: Technical File PPE Marking section.

EHSR Ref 1.3.3, 2.4, 2.12;

The information supplied by the manufacturer is defined in the relevant section of the technical file. This information includes explanation required by all applied product standard requirements. The defined user information text in the technical file includes the following data;

Article 7

- Name / trademark of the manufacturer, its address, or the authorised representative for EU community
- Type of protection against chemicals (Type-6). The information also includes a reminder for wearing necessary additional PPE in order to achieve a full body protection (i.e boots, gloves, mask and visor / face shield).
- Size of the coverall and model name
- The standard code / name with the published year
- The statement that the coverall is tested against the chemical names (tested for) and performance levels for mechanical strengths including repellency and resistance to penetration of liquids (Based on EN 14325:2018 classification)
- Pictogram and information that the PPE is non-reusable also the shelf life is mentioned

EN ISO 13034:2005 + A1:2009 Standard Requirements Evaluation

- Instructions for use, controls before use, how to wear / unwear, limitations, instructions for storage conditions, complementary, instructions for disposal
- The statement on the light spray test results
- Statement for warning the user on flammability, to keep away of fire

The above user information text is available in Turkish  
Ref Technical File, User Information Sheet

ESSENTIAL HEALTH and SAFETY REQUIREMENTS GIVEN IN EUROPEAN UNION REGULATION EU  
2016/425 CORRESPONDING to Annex ZA of EN ISO 14126:2003 + AC:2004 STANDARD

**1. GENERAL REQUIREMENTS APPLICABLE TO ALL PPE**

**1.1. Design principles**

**1.1.2.2. Classes of protection appropriate to different levels of risk**

Where differing foreseeable conditions of use are such that several levels of the same risk can be distinguished, appropriate classes of protection must be taken into account in the design of the PPE.

**1.3. Comfort and effectiveness**

**1.3.1. Adaptation of PPE to user morphology**

PPE must be designed and manufactured in such a way as to facilitate its correct positioning on the user and to remain in place for the foreseeable period of use, bearing in mind ambient factors, the actions to be carried out and the postures to be adopted. For this purpose, it must be possible to adapt the PPE to fit the morphology of the user by all appropriate means, such as adequate adjustment and attachment systems or the provision of an adequate range of sizes.

**1.3.2. Lightness and strength**

PPE must be as light as possible without prejudicing its strength and effectiveness.

PPE must satisfy the specific additional requirements in order to provide adequate protection against the risks for which it is intended and PPE must be capable of withstanding environmental factors in the foreseeable conditions of use.

**1.4. Manufacturer's instructions and information**

In addition to the name and address of the manufacturer, the instructions that must be supplied with the PPE must contain all relevant information on:

- instructions for storage, use, cleaning, maintenance, servicing and disinfection. Cleaning, maintenance or disinfectant products recommended by manufacturers must have no adverse effect on the PPE or the user when applied in accordance with the relevant instructions;
- performance as recorded during relevant technical tests to check the levels or classes of protection provided by the PPE;
- where applicable, accessories that may be used with the PPE and the characteristics of appropriate spare parts;
- where applicable, the classes of protection appropriate to different levels of risk and the corresponding limits of use;
- where applicable, the month and year or period of obsolescence of the PPE or of certain of its components;
- where applicable, the type of packaging suitable for transport;
- the significance of any markings (see point 2.12);
- the risk against which the PPE is designed to protect;
- the reference to this Regulation and, where applicable, the references to other Union harmonisation legislation;
- the name, address and identification number of the notified body or bodies involved in the conformity assessment of the PPE;
- references to the relevant harmonised standard(s) used, including the date of the standard(s), or references to the other technical specifications used;
- the internet address where the EU declaration of conformity can be accessed.

The information referred to in points (i), (j), (k) and (l) need not be contained in the instructions supplied by the manufacturer if the EU declaration of conformity accompanies the PPE.

**2. ADDITIONAL REQUIREMENTS COMMON TO SEVERAL TYPES OF PPE**

**2.4. PPE subject to ageing**

If it is known that the design performance of new PPE may be significantly affected by ageing, the month and year of manufacture and/or, if possible, the month and year of obsolescence must be indelibly and unambiguously marked on each item of PPE placed on the market and on its packaging.

If the manufacturer is unable to give an undertaking with regard to the useful life of the PPE, his instructions must provide all the information necessary to enable the purchaser or user to establish a reasonable obsolescence month and year, taking into account the quality level of the model and the effective conditions of storage, use, cleaning, servicing and maintenance.

Where appreciable and rapid deterioration in PPE performance is likely to be caused by ageing resulting from the periodic use of a cleaning process recommended by the manufacturer, the latter must, if possible, affix a marking to each item of PPE placed on the market indicating the maximum number of cleaning operations that may be carried out before the equipment needs to be inspected or discarded. Where such a marking is not affixed, the manufacturer must give that information in his instructions.

**2.12. PPE bearing one or more identification markings or indicators directly or indirectly relating to health and safety**

Where PPE bears one or more identification markings or indicators directly or indirectly relating to health and safety, those identification markings or indicators must, if possible, take the form of harmonised pictograms or ideograms. They must be perfectly visible and legible and remain so throughout the foreseeable useful life of the PPE. In addition, those markings must be complete, precise and comprehensible so as to prevent any misinterpretation. In particular, where such markings include words or sentences, the latter must be written in a language easily understood by consumers and other end-users, as determined by the Member State where the PPE is made available on the market.

Where PPE is too small to allow all or part of the necessary marking to be affixed, the relevant information must be mentioned on the packaging and in the manufacturer's instructions.

**3. ADDITIONAL REQUIREMENTS SPECIFIC TO PARTICULAR RISKS**

**3.10. Protection against substances and mixtures which are hazardous to health and against harmful biological agents**

**3.10.2. Protection against cutaneous and ocular contact**

PPE intended to prevent the surface contact of all or part of the body with substances and mixtures which are hazardous to health or with harmful biological agents must be capable of preventing the penetration or permeation of such substances and mixtures and agents through the protective integument under the foreseeable conditions of use for which the PPE is intended.

To this end, the constituent materials and other components of those types of PPE must be chosen or designed and incorporated so as to ensure, as far as possible, complete leak-tightness, which will allow where necessary prolonged daily use or, failing this, limited leak-tightness necessitating a restriction of the period of wear.

Where, by virtue of their nature and the foreseeable conditions of their use, certain substances and mixtures which are hazardous to health or harmful biological agents possess high penetrative power which limits the duration of the protection provided by the PPE in question, the latter must be subjected to standard tests with a view to their classification on the basis of their performance. PPE which is considered to be in conformity with the test specifications must bear a marking indicating, in particular, the names or, in the absence of the names, the codes of the substances used in the tests and the corresponding standard period of protection. The manufacturer's instructions must also contain, in particular, an explanation of the codes (if necessary), a detailed description of the standard tests and all appropriate information for the determination of the maximum permissible period of wear under the different foreseeable conditions of use.

Technical Assessment of EN 14126:2003 + AC:2004 Standard and other Standards it refers to, Clauses Corresponding to the Essential Health and Safety Requirements given above

**EN 14126:2003 + AC:2004 Standard Requirements Evaluation**

*Article 4.1.2*  
EHSR Ref 1.3.2;  
The overall material performance are tested according to EN 14325:2018 standard for the relevant properties required by the Type defining standards for protective clothing. The overall under evaluation claims compliance with Type 5, Type 6. The required mechanical and flammability performance levels are evaluated in the corresponding clauses of EN ISO 13034:2005 + A1:2009 standard within this report. No further evaluation is necessary for this standard.

*Article 4.1.4*  
EHSR Ref 1.1.2.2, 3.10.2;  
Evaluation of the performance requirements against penetration by inactive agents;  
The overall is subjected to the tests according to ISO 16603 and ISO 16604 standards for its resistance to penetration by contaminated liquids under hydrostatic pressure. According to the obtained results of the corresponding test report;

- The overall material with stands and do not allow any penetration of bacteria under 20kPa hydrostatic pressure and is classified as **Class 6** according to Table 1 given in 4.1.4.1 Clause of this standard,
- The overall material was also subjected to evaluation of the bacteriophage test and passes the test according to ISO 16604 at 20kPa, and is classified as **Class 6** according to Table 1 given in 4.1.4.1 Clause of this standard,

The overall is tested for its resistance to penetration by infective agents due to mechanical contact with substances containing contaminated liquids according to ISO 22610:2018 testing standard. The laboratory environmental conditions and the test setup parameters were inline with the standard requirements. The laboratory results indicates that the tested specimens allows penetration in first 15 minutes and classified as **Class 1** according to Table 2 of Clause 4.1.4.2 of EN 14126 standard Classification of resistance to penetration by infective agents due to mechanical contact with substances containing contaminated liquids.

The overall is tested for its resistance to penetration by contaminated solid particles according to ISO 22612:2005 testing standard. The laboratory environmental conditions and the test setup parameters were inline with the standard requirements. The laboratory results indicates that the tested 10 specimens the arithmetic mean of penetration results are smaller than 2 log cfu. The tested sample is classified as **Class 2** according to Table 4 of Clause 4.1.4.4 of EN 14126 standard Classification of resistance to penetration by contaminated solid particles.

The results of evaluation for clause 4.1.4 is summarised below;

Resistance to Penetration Property	Result Classification		Requirement of EN 14126
	Classification	Result	
ISO 16604 - Resistance to penetration by contaminated liquids under hydrostatic pressure	Class 6	Successful Hydrostatic pressure > 20 kPa	To be Classified
EN ISO 22610 - Resistance to penetration by infective agents due to mechanical contact with substances containing contaminated liquids.	Class 1	Breakthrough time t < 15min	To be Classified
EN ISO 22612 - Resistance to penetration by contaminated solid particles	Class 2	Penetration 1 < log cfu ≤ 2	To be Classified

Ref: Laboratory Test Report 4

**EN 14126:2003 + AC:2004 Standard Requirements Evaluation**

<i>Article 4.2</i>	<p>EHSR Ref 1.3.2;</p> <p>The seam strength is evaluated and classified based on the test report as shown below;</p> <table border="1" style="width: 100%;"> <thead> <tr> <th>Property of Material EN 14325:2018</th> <th>Result Classification</th> <th>Requirement of EN 14126</th> </tr> </thead> <tbody> <tr> <td>5.5 Seam Strength</td> <td>Refer to the strength values for seams at different parts of coverall. The lowest Class is given among all kinds of seams Class 1</td> <td>To be Classified</td> </tr> </tbody> </table> <p>Ref: Laboratory Test Report 1</p>	Property of Material EN 14325:2018	Result Classification	Requirement of EN 14126	5.5 Seam Strength	Refer to the strength values for seams at different parts of coverall. The lowest Class is given among all kinds of seams Class 1	To be Classified
Property of Material EN 14325:2018	Result Classification	Requirement of EN 14126					
5.5 Seam Strength	Refer to the strength values for seams at different parts of coverall. The lowest Class is given among all kinds of seams Class 1	To be Classified					
<i>Article 4.3</i>	<p>EHSR Ref 1.3.1, 3.10.2;</p> <p>The PPE under evaluation conforms the relevant requirements of EN ISO 13688 standard. The requirements of the coverall with respect to health and safety, ageing and sizing are evaluated in EN ISO 13688 section of this report.</p>						
<i>Article 5</i>	<p>EHSR Ref 2.12;</p> <p>The marking requirements for protective clothing against chemicals are evaluated in the relevant section of this report. Additionally;</p> <p>Each piece of coverall have marking with the following information on the single PPE package / PPE itself;</p> <ul style="list-style-type: none"> <li>• Applied product standards (EN 14126:2003+AC:2004)</li> <li>• Type marking of the PPE as Type 5-B / Type 6-B</li> <li>• the pictogram "protection against biological hazard"</li> </ul> <p>The above mentioned marking requirements are stated in the technical file of the manufacturer. The evaluated samples did not have all these marking and information on the PPE. The manufacturer shall follow the instructions in the technical file in case of serial manufacturing of the PPE and verify before putting the PPE on the market.</p> <p>Ref: Technical File PPE Marking Section</p>						
<i>Article 6</i>	<p>EHSR Ref 1.4;</p> <p>The information supplied by the manufacturer is defined in the relevant section of the technical file. This information includes explanation required by all applied product standard requirements. The defined user information text in the technical file includes the following data;</p> <ul style="list-style-type: none"> <li>• Name / trademark of the manufacturer, its address, or the authorised representative for EU community</li> <li>• Type of protection against chemicals (Type 5-6). The information also includes a reminder for wearing necessary additional PPE in order to achieve a full body protection (i.e boots, gloves, mask and visor / face shield).</li> <li>• The standard number (EN 14126)</li> <li>• The performance levels identified with the tests against inactive agents</li> <li>• Pictogram and information that the PPE is non-reusable also the shelf life is mentioned</li> <li>• Instructions for use, controls before use, how to wear / unwear, limitations, instructions for storage conditions, complementary, instructions for disposal</li> </ul> <p>The above user information text is available in Turkish. Ref User Information Sheet</p>						





**Sample Photos**



PPE Experts contributed to this report:

Arzu ŞEREMETLİ

Osman CAMCI

Approval  
Suat KAÇMAZ  
UNIVERSAL CERTIFICATION – Director

**Müşterinin adı:** UNIVERSAL SERTİFİKASYON VE GÖZETİM HİZMETLERİ TİCARET LTD.ŞTİ.  
**Adresi:** NECİP FAZIL BULVARI KEYAP SİTESİ E2 ÜMRANIYE/İSTANBUL  
**Alıcı firma:** YALITKAN PASPAS KAUÇUK ÜRÜNLERİ A.Ş.  
**İlgili kişi:** SUAT KAÇMAZ  
**İstek numarası:** -  
**Model numarası:** -  
**Numunenin adı ve tarifi:** Beyaz tulum  
**Numunenin kabul tarihi:** 06.11.2020  
**İlave numune ve/veya ilave bilgi geliş tarihi:** -  
**Deneyin yapıldığı tarih:** 06.11.2020-12.11.2020  
**Açıklamalar:** -  
**Numune alımı:** Bu raporda verilen sonuçlar müşteri tarafından gönderilen numuneye aittir.  
**Numunenin son kullanımı:** -  
**Yıkama talimatı:** Belirtilmedi.  
**Raporun sayfa sayısı:** 8

Türk Akreditasyon Kurumu (TÜRKAK) deney raporlarının tanınması konusunda Avrupa Akreditasyon Birliği (EA) ve Uluslararası Laboratuvar Akreditasyon Birliği (ILAC) ile karşılıklı tanıma anlaşmasını imzalamıştır. Deney laboratuvarı olarak faaliyet gösteren EKOTEKS LABORATUVAR ve GÖZETİM HİZMETLERİ A.Ş. TÜRKAK'tan AB-0583-T akreditasyon dosya numarası ile ISO 17025:2017 standardına göre akredite edilmiştir. Deney ve/veya ölçüm sonuçları, genişletilmiş ölçüm belirsizlikleri (olması halinde) ve deney metodları bu sertifikasyon tamamlayıcı kısmı olan takip eden sayfalarda verilmiştir.



Tarih  
12.11.2020

Müşteri Temsilcisi  
YESİM ŞAHİN

Laboratuvar Müdürü  
Sevim A. BAZAK  
12.11.2020

Bu rapor, laboratuvarın yazılı izni olmadan kısmen kopyalanıp çoğaltılamaz.  
İmzasız ve mühürlü raporlar geçersizdir.

İSTENEN TESTLER	SONUÇ	AÇIKLAMA
<b>FİZİKSEL TESTLER</b>		
Aşınma	-	Sınıf 6
Su Geçirgenliği	-	Sınıf 6
Yırtılma Mukavemeti	-	Sınıf 2
Kopma Mukavemeti	-	Sınıf 2
Sıvılara Karşı İticecilik	-	Sınıf 3
Sıvıların Nüfus Etmesine Karşı Direnci	-	Sınıf 3
Dikiş Mukavemeti	-	Sınıf 2
Delinme Dayanımı	-	Sınıf 1
Esnetme ile oluşan hasara karşı direncin Tayini	-	Sınıf 3
Yanmazlık	P	Sınıf 1
P:Geçer F:Kalır R:Alıcı firmanın teknik kişisine başvurunuz. Test sonuçları BS EN 14325:2018'e göre sınıflandırılmıştır. (Referans Standart BS EN 14126 :2003 Enfekte Edici Ajanlara Karşı Koruyucu Giyecekler –Performans Özellikleri ve Deney Metotları) <sup>(1)</sup> İstenen değerler müşteri tarafından belirtilmemiştir		

Not: Aksi belirtilmediği takdirde testler ile ilgili kayıtlar 5 yıl, orjinal numuneler 3 ay saklanır. Müşteri tarafından talep edildiğinde testlere ait ölçüm belirsizliği raporlanır fakat "Geçer/Kalır" değerlendirilmesinde ölçüm belirsizliği değeri dikkate alınmaz. Raporlanan belirsizlik, genişletilmiş belirsizlik olup standart belirsizlik kapsam faktörü k=2 kullanılarak elde edilmiştir. Güvenilirlik düzeyi % 95'tir. Uygunluk beyanı Basit Kabul Karar Kuralına göre verilmiştir. Bu raporda (\*) işaretli deneyler akreditasyon kapsamına dahil değildir.



This report shall not be reproduced other than in full except with the permission of the laboratory.  
Testing reports without signature and seal are not valid.

AB-0583-T

20041658

11-20

## TEST SONUÇLARI

### YIRTILMA MUKAVEMETİ;

**Madde 4.7.Trapezoidal Yırtılma Dayanımı** TS EN ISO 9073-4:2002

Instron 5969 Hız: 100 mm/dk±10, Çene mesafesi 5 cm.  
En boy yönlerinde 4 adet sonucun ortalaması verilmiştir.  
2N Ön gerilim uygulanmıştır.  
Kondüsyon şartlarında test edilmiştir. (20±2°C - %65±4)

	<b>SONUC</b>
Atkı	54.63 N
Çözüğü	27.81 N

**SINIF**  
2

Tablo-4 'e göre yapılır

### Yırtılma Dayanımının Sınıflandırılması (Tablo-4)

Sınıf	Yırtılma Mukavemeti
6	>150 N
5	>100 N
4	>60 N
3	>40 N
2	>20 N
1	>10 N

### KOPMA MUKAVEMETİ;

**Madde 4.9.Kopma Mukavemeti** EN ISO 13934-1:2013

Hız: 100 mm/dk±10, Çene mesafesi 200 mm.  
Ön gerilme uygulanmamıştır. İslatma işlemi yapılmamıştır.  
Atkı ve Çözüğü yönlerinde 4 adet sonucun ortalaması verilmiştir.  
Kondüsyon şartlarında test edilmiştir. (20±2°C - %65±4)

	<b>SONUC</b>
EN	115.7 N

**SINIF**  
2

Tablo-5 'e göre yapılır

**BOY** 46.5 N

### Kopma Mukavemeti Sınıflandırılması (Tablo-5)

Sınıf	Kopma Mukavemeti
6	>1000 N
5	>500 N
4	>250 N
3	>100 N
2	>60 N
1	>30N

AB-0583-T

20041658

11-20

## TEST SONUÇLARI

**Test Metodu: BS EN 14325:2018 ( KIMYASALLARA KARŞI KORUYUCU GIYSİLER- KIMYASAL KORUYUCU GIYSİ MALZEMELERİNİN, DİKİŞLERİN VE BİRLEŞTİRİCİ MALZEMELERİN PERFORMANS SINIFLANDIRILMASI VE TEST METOTLARI)**

### AŞINMA DAYANIMI ve SIZDIRMAZLIK

**Madde 4.4.Aşınma Dayanımı (EN ISO 12947-2) EK-B**

Lissajous deseni oluşturan Martindale Test Cihazı (47.5±2 rpm)  
9 kPa basınç. (595±7) g kütle.  
Kondüsyon şartlarında test edilmiştir.(20±2°C-65%±4)

**SONUC**

Aşınmadı @ 2.000 devir

**SINIF**  
6

Tablo-1 'e göre yapılır

Malzemeye zarar vermeyen en yüksek aşınma devri Tablo-1 e göre tayin edilir.  
Aşınma Dayanımının Sınıflandırılması (Tablo-1)

Sınıf	Devir Sayısı
6	>2000
5	>1000
4	>400
3	>100
2	>40
1	>10

**Madde 4.4.2.3 Su geçirmezlik tayini hidrostatik basınç metodu (EN 20811)**

Orijinal numune ( aşındırılmamış) test sonucu > 200 mmSS olmalıdır.Bunu sağlarsa madde 4.4'e göre en yüksek devirde bulunan numuneye EN 20811 uygulanır.

### SU GEÇİRGENLİĞİ; EN ISO 20811:2018

Hidrostatik Başlık Cihazı, Textest marka Fx 3000 model  
Su sıcaklığı 10 .°C. Basınç artış oranı 10 mbar/dk.  
Kondüsyonlu ortamda test edilmiştir. (20±2°C-65%±4).

	<b>SONUC</b>
Numune 1	399,8 mm SS
Numune 2	465,12 mm SS
Numune 3	482,4 mm SS
Ortalama	445,1 mm SS

**İSTENEN**  
>200 mmSS



## TEST SONUÇLARI SIVILARA KARŞI İTİCİLİK ÖZELLİĞİ

### Madde 4.12 Sıvılara Karşı İtıcilik (EN ISO 6530:2005)

Sıvı dayanımı Tablo-9 da verilen sıvı kimyasallar yada genel amaçlı bir izlenimi görmek için test sıvısı olarak su da kullanılabilir. Kondüsyon şartlarında test edilmiştir. (20±2°C - %65±4)  
Test edilecek herbir kimyasal sıvıya dayanımı ölçmek için 3 en, 3 boy numune (360±2)mm x (235±5)mm alınmıştır. Analitik saflıkta kimyasal kullanılmıştır. Test sıvısı (10cm<sup>3</sup>), (10±1)s de numune yüzeyinden geçirilmiştir. Bkz Tablo-9 Sonuç Değerlendirmesi Tablo-10 ve tbalo-11'e göre yapılmıştır.

Absorbsiyon, Penetrasyon (nüfus etme) ve iticilik testlerinde kullanılan kimyasallar (Tablo-9)

Kimyasal	Kimyasal Marka	% Konsantrasyon	Sıcaklık ( ±2°C)
Sülfürik Asit (H <sub>2</sub> SO <sub>4</sub> )		30	20
Sodyum Hidroksit (NaOH)		10	20
o-Xylene		Seyreltik değil	20

Sıvı İtıciliğinin Sınıflandırılması (Tablo-10)

Sınıf	İtıcilik İndeksi (IR)
3	> 90 %
2	>80 %
1	>70 %

### Madde 4.13 Sıvıların Nüfus Etmesine Karşı Direnci (EN ISO 6530)

Sıvılara Karşı Nüfus Etme Direncinin Sınıflandırılması (Tablo-11)

Sınıf	Nüfus Etme İndeksi (Ip)
3	< 1 %
2	< 5 %
1	<10 %

## SONUC

Kimyasal	%Konsantrasyon	I <sub>p</sub>	Sınıf	I <sub>R</sub>	Sınıf
Sülfürik Asit (H <sub>2</sub> SO <sub>4</sub> )	30	% 0	3	% 96,33	3
Sodyum Hidroksit (NaOH)	10	% 0	3	%96,16	3
o-Xylene	Seyreltik değil	% 0	3	%94,01	3

## TEST SONUÇLARI

### DİKİŞ MUKAVEMETİ-GRAB METOT ;

Madde 5.5 Dikiş Mukavemeti ISO 13935-2: 2014

NSTRON 5969

Hız: 50±5 mm/dk. Çene Aralığı: 100 ±1 mm

5KN yük uygulanmıştır.

Kondüsyon şartlarında test edilmiştir. ( 20±2°C-65%±4 )

	Dikiş Mukavemeti (N)	Hata	SINIFLANDIRMA
Kol dikişi	75.03 N	FTJ	Sınıf 2 Tablo-13 'e göre yapılıdır
Şapka	73.06 N	FTJ	
Elcik	55.81 N	FTJ	
Ağ	107.54 N	FR	
İç yan	126.37 N	FTJ	
Ön orta	109.26 N	FTS	
Arka orta	140.98 N	FTJ	
Bel	78.32 N	FTJ	

FTJ : Çenede Kumaş Yırtılması

Dikiş Mukavemeti Sınıflandırılması (Tablo-13)

SINIF	Dikiş Mukavemeti
6	>500 N
5	>300 N
4	>125 N
3	>75 N
2	>50 N
1	>30 N

AB-0583-T

20041658

11-20

## TEST SONUÇLARI

### DELİNME DAYANIMI

Madde 4.10. Delinme Dayanımı EN 863 : 1995

#### SONUÇ

6.5 N

#### SINIF

1  
Tablo-6 'ya göre  
yapılır

Delinme Dayanımının Sınıflandırılması (Tablo-6)

Sınıf	Delinme Dayanımı
6	>250 N
5	>150 N
4	>100 N
3	>50 N
2	>10 N
1	>5N

AB-0583-T

20041658

11-20

## TEST SONUÇLARI

### ESNETME İLE OLUŞAN HASARA KARŞI DİRENCİN TAYİNİ METOT C (BÜKÜLME /ESNEKLİK TESTİ) Madde 4.5

Test Metodu : ISO 7854 : 1995 Kauçuk veya Plastik Kaplı Kumaşlar –  
Esnetme ile oluşan hasara karşı direncin tayini Metot C (Bükülme /Esneklik Test) (\*)  
220 mm boy x 190 mm en ebatlarında 2 numune hazırlanır.  
Devir tamamlanınca varsa hasar tespit edilir ve sınıflandırma Tablo 2 ye göre yapılır.

#### SONUÇ

>5 000devir

Hasar gözlenmemiştir.

#### SINIF

Sınıf 3  
Tablo-2' e göre yapılır

Tablo-2 Bükülme ve Esneklik Direncinin Sınıflandırılması

Sınıf	Devir Sayısı
6	> 100 000
5	>40 000
4	> 15 000
3	> 5 000
2	> 2 500
1	> 1000

## YANMAZLIK ;

BS EN 14325:2018 Madde 4.14 (Tutuşmaya Karşı Dayanım)  
(Ref: BS EN 13274-4:2001- METOT 3

Kondüsyonlama	65±5 % RH, 20±2°C/24 saat
Test Atmosferi	16-32° (±1°C)
Alev Yüksekliği	40± 2 mm
Gaz Tipi	Propan (min %95 saflıkta)
Alev Sıcaklığı	800±50°C
Test Edilen Numune Boyutu	560 x 170 (boy x en)
Numune Hareket Hızı	60 ± 5 mm/s.
SONUÇ	Level 1
İSTENEN	Numune alevin içinden hiç durmadan geçer

GCNTR ULUSLARARASI BELGELENDİRME, GÖZETİM, EĞİTİM VE DIŞ TİC. LTD. ŞTİ.  
Atak Plaza-Tavukçuyolu Cad. Demirtürk Sok. No:10 Yukari Dudullu Umraniye, İstanbul / TURKEY

### TEST REPORT

Report Date: 12.11.2020  
Report Number: GTL-TLM-0078A/20

#### CLIENT and SAMPLE INFORMATION

TEST OWNER	UNIVERSAL CERTIFICATION and SURVEILLANCE SERVICES TRADE CO		
ADDRESS	Necip Fazil Bulvarı Keyap Sitesi E2 Blok No:44/84 Yukari Dudullu Umraniye, İstanbul / TURKEY		
MANUFACTURER	YALITKAN PASPAS KAUÇUK ÜRÜNLERİ A.Ş		
ADDRESS	ORUÇREİS MAH. TEKSTİL KENT CAD. GD1 BLOK NO:148 ESENLER/İSTANBUL		
SAMPLE DESCRIPTION	Protective Clothes		
BRAND NAME - MODEL	-		
TESTING STANDARD	EN 13982-1:2018		
SAMPLE RECEIVE DATE	06.11.2020	TESTING START DATE	10.11.2020

The results given in this test report belongs to the samples tested. The report content cannot be recreated partially without the written consent of GCNTURK.



Mr. Sebahattin ÇAY  
General Coordinator

#### 1. REPORT SUMMARY

TEST STANDARD	TEST NAME	RESULT
EN 13982-1:2018 clause 4.3.2 ISO 13982-2	Inward Leakage Testing	Pass



## 2. TEST RESULTS and EVALUATION

### 4.3.2 Inward leakage of aerosols of solid particles

**Test Method:** ISO 13982-2

Temperature and relative humidity measurements were recorded in the test chamber immediately after each test and these ranged from 20.2 to 22.5 °C and 30.2 to 34.8%, respectively

Before testing a suit according to ISO 13982-2, the subject shall be except that he must repeat the following three rows of moves three times:

- Movement 1: Both knees collapse, lean forward and hands are placed on the floor at a distance of 45 cm from the front of the knees. It is crawled forward on the hands and knees for 3 m and the same distance is crawled back again.

- Movement 2: Standing with feet wide and arms on the side. Arms in front of the body

It is removed until it is parallel to the ground. It crouches down as much as possible.

- Movement 3: Kneel down on the right knee, knee bent 90° and place the left foot on the ground, hang loosely from the edge with the left arm. The left arm is lifted completely over the head

REQUIREMENT	RESULTS	COMMENT
Ljmn,82/90 ≤ % 30, LS,8/10 ≤ % 15.	Pass	Detail refer to Annex I In response to the question "does the suit fit", all test subjects answered "Yes". After testing in accordance with the movements defined in clause 4.3.2 of EN 13982-1: 2018, no damage to the suit was observed.



### Annex I-Test Result:

Table I NaCl inward leakage (%) individual results

Wearer	Position	Knee	Waist back	Chest	Average
1	Stand	10,05	9,70	12,05	10,60
	Walk	11,03	9,60	13,70	11,44
	Squat	10,90	12,30	12,10	11,77
	Average	10,66	10,53	12,62	11,27
1	Stand	15,60	9,73	9,01	11,45
	Walk	9,94	9,16	12,45	10,52
	Squat	10,35	10,00	10,60	10,31
	Average	11,96	9,63	10,69	10,76
2	Stand	12,56	10,29	10,93	11,26
	Walk	10,20	16,48	12,63	13,10
	Squat	10,47	9,95	10,39	10,27
	Average	11,08	12,24	11,32	11,55
2	Stand	9,50	8,42	9,32	9,08
	Walk	10,21	9,94	9,59	9,91
	Squat	10,24	9,92	10,29	10,15
	Average	9,98	9,42	9,73	9,71
3	Stand	9,80	8,67	9,56	9,34
	Walk	10,22	10,23	9,82	10,09
	Squat	10,50	10,05	10,47	10,34
	Average	10,17	9,65	9,95	9,92
3	Stand	10,02	9,02	9,66	9,57
	Walk	10,08	10,19	10,20	10,16
	Squat	10,47	10,11	10,70	10,43
	Average	10,28	9,77	10,19	10,06
4	Stand	10,10	9,37	9,56	9,68
	Walk	9,92	10,16	10,51	10,20
	Squat	10,31	10,24	10,60	10,38
	Average	10,11	9,92	10,22	10,09
4	Stand	10,83	9,77	9,90	10,17
	Walk	10,30	10,57	10,47	10,45
	Squat	10,61	10,24	10,64	10,50
	Average	10,58	10,19	10,34	10,37
5	Stand	9,97	10,52	7,21	9,24
	Walk	9,31	8,69	6,63	8,21
	Squat	12,60	10,94	9,42	10,99
	Average	10,63	10,05	7,76	9,48
5	Stand	10,24	8,54	9,29	9,36
	Walk	12,05	11,01	8,69	10,58
	Squat	9,75	8,79	11,35	9,96
	Average	10,68	9,45	9,78	9,97



Table 2: Total inward leakage (%) (overall average, all wearers)

Position	Knee	Waist back	Chest	Average
Stand	10,87	9,40	9,65	9,97
Walk	10,37	10,60	10,47	10,48
Squat	10,62	10,25	10,66	10,51
Average	10,62	10,09	10,26	10,32

Table 3: Total inward leakage per test subject

Wearer	Average
1	11,01
2	10,63
3	9,99
4	10,23
5	9,72
Average	10,32

The physical dimensions of the wearers are shown below:

Wearer	Height (cm)	Chest (cm)	Suit size
1	182	104	-
2	183	99	-
3	182	95	-
4	186	98	-
5	184	97	-

Pass	Requirement satisfied.
NCR	Requirement not satisfied. Refer to the "Result details" section for more information.
NAs	Assessment not carried out.
N/A	Requirement not applicable.

Sample Photo



- End of Report -

Test Report

**Test Owner name / address** UNIVERSAL CERTIFICATION and SURVEILLANCE SERVICES TRADE CO.  
Necip Fazıl Bulvarı Keyap Sitesi E2 Blok No:44/84 Yukari Dudullu Umraniye, Istanbul /  
TURKEY

**Manufacturer name/address** YALITKAN PASPAS KAÇUK ÜRÜNLERİ A.Ş  
ORUÇREİS MAH. TEKSTİLKENT CAD. GD1 BLOK NO:148 ESENLER/İSTANBUL

**Name and identity of the test item** Protective Clothes

**The date of receipt of the test item** 06.11.2020

**Brand name – model** -

**Date of the test** 10.09.2020

**Sample Number** GTTS-0078-1, GTTS-0078-2, GTTS-0078-3


**Number of pages of the report** 8

GCNTR ULUS.BELG.GÖZ.EĞT.VE DIŞ.TİC.LTD.ŞTİ accredited by TÜRKAK under registration number AB-1272-T for EN ISO17025 as test laboratory\*.  
The test and/or measurement results, the uncertainties (if applicable) with confidence probability and test methods are given on the following pages which are part of this report.

Date/Seal  
12.11.2020



Head of Testing Laboratory  
Sebahattin ÇAY



This report only applies to the sample tested.  
This report shall not be reproduced other than in full except with the permission of the laboratory Testing reports without signature and seal are not valid

Report No: **GTL-TLM-0078/20**

Test Report

Contents

1. Documentation .....	3
1.1 Description of the EUT.....	3
1.2 Environmental Condition, Symbol Definitions.....	3
1.3 Test Standards .....	3
2. Test Result .....	4
3. Attachments .....	7
3.1 Photos of EUT .....	7



This report only applies to the sample tested.  
This report shall not be reproduced other than in full except with the permission of the laboratory Testing reports without signature and seal are not valid

Report No: **GTL-TLM-0078/20**

Test Report

1. Documentation

1.1 Description of the EUT

All samples tested

Test samples subject to the test

Product Name	Samples No	Sample Size	Type	Application Tests
Protective Clothing	GTTS-0078-1	L	Type 6	Pre-exercise Test- Spray Test
Protective Clothing	GTTS-0078-2	L	Type 6	Pre-exercise Test- Spray Test
Protective Clothing	GTTS-0078-3	L	Type 6	Pre-exercise Test-Spray Test

1.2 Environmental Condition, Symbol Definitions

- Test case does not apply to the test object .....: N/A
- Test object meets the requirement.....: P (Pass)
- Test object does not meet the requirement.... : F (Fail)
- Environmental Conditions: °C ,% RH, m/s

1.3 Test Standards

EN 13034+A1:2011 Protective clothing against liquid chemicals – Performance requirements for chemical protective clothing offering limited protective performance against liquid chemicals (Type 6 and Type PB [6] equipment).

EN ISO 17491-4 protective clothing – test methods for clothing providing protection against chemical – part 4: Determination of resistance to penetration by a spray of liquid (spray test)



Test Report

2. Test Result

Clause	Requirement	Result – Remark	Verdict
--------	-------------	-----------------	---------

TS EN 14325 4.2	<b>Pre-Treatment</b>		
TS EN 14325 Article 4.2.1	Prior to testing, the chemical protective clothing shall be cleaned, if the manufacturer's instructions indicate that cleaning is allowed. Manufacturer's instructions with regard to number of cleaning cycles, cleaning procedures and possible reapplication of treatments shall be observed. If no maximum number of cleaning cycles is indicated, the clothing shall undergo five cleaning cycles.	Protective clothing are, it's was come in the form of plastic packing by the company. For this reason, no additional cleaning was performed with the suggestion of the company.	PASS
TS EN 14325 4.3	<b>Conditioning</b>		
	All chemical protective clothing shall be conditioned for at least 24 h at the same conditions as used for the test.	All products are conditioned at 24 C° 50% Rh values for 24 hours.	PASS
TS EN 13034+A1 5.2	<b>Pre-Test</b>		
		In the exercise test deformations were. Deformation details is given in the figure 1.	PASS
TS EN 13034+A1 5.2	<b>Resistance to the penetration of liquids (SprayTest)</b>	<b>Type 6</b>	
EN ISO 17491-4 Article 9	Remove respirator and gloves first before opening the test garment. Remove the chemical protective clothing carefully in order to avoid contamination of the absorbent overall and examine the internal surface of the test garment for signs of penetration, paying special attention to openings, seams, closures and zippers. Mark them.	Three test clothes were dressed tested together with the white absorbent underwear.  Region passing of liquid are given in figure 1.	PASS
TS EN 13034+A1 Article 5.2	Any underwear, of each garment suit The total stain area on it should not be more than three times the calibrated total stain area.	Calibration stain area: measured as 4.56 cm².  sum of stains on the inner white garment are given in table 2	PASS

Test Report

Table 1

Clause	Requirement	Pre-Experiment		Liquid Experiment 1		Liquid Experiment 2		Liquid Experiment 3	
		PASS	FAIL	PASS	FAIL	PASS	FAIL	PASS	FAIL
	Starting from a standing position in each case, carry out the following movement sequence:								
Movement 1	Kneel on both knees, lean forward and place both hands on the floor ( $45 \pm 5$ ) cm in front of the knees; crawl forward and backwards on hands and knees for a distance of three metres in each direction;	✓		✓		✓		✓	
Movement 2	Climb a vertical ladder at least four steps, rungs to be as encountered on a typical ladder;	✓		✓		✓		✓	
Movement 3	Position hands at chest level, palms out; reach directly overhead, interlock thumbs, extend arms fully upwards;	✓		✓		✓		✓	
Movement 4	Kneel on right knee, place left foot on floor with left knee bent ( $90 \pm 10$ )°; touch thumb of right hand to toe of left shoe. Repeat movement with alternate posture, i.e. by kneeling on left knee and placing the right foot on the floor with knee bent at 90°.	✓		✓		✓		✓	
Movement 5	Extend arms fully in front of body, lock thumbs together, twist upper body ( $90 \pm 10$ )° left and right;	✓		✓		✓		✓	
Movement 6	Stand with feet shoulder width apart, arms at side; raise arms until they are parallel to the floor in front of the body; squat down as far as possible;	✓		✓		✓		✓	
Movement 7	Kneel as in movement 4, left arm hanging loosely at side; raise arm fully overhead. Repeat movement with alternate posture by alternating arms.	✓		✓		✓		✓	

Test Report

Pre-experiment 1	M.A Height: 170 cm Weight: 70 kg
Liquid Experiment 1	M.A
Liquid Experiment 2	M.A
Liquid Experiment 3	M.A

Table 2

	SPREY EXPERIENCE					SUM
	UPPER BODY			LOWER BODY		
	Chest (cm <sup>2</sup> )	Shoulder (cm <sup>2</sup> )	Back (cm <sup>2</sup> )	Front (cm <sup>2</sup> )	Back (cm <sup>2</sup> )	
GTTS-0078						
Sample 1	-	-	-	-	-	0
Sample 2	-	-	-	-	-	0
Sample 3	1,3	0,8	1,7	-	-	3,8



GTL-TLM-0078/20

12.11.2020

Test Report

3. Attachments

3.1 Photos of EUT



Report No: GTL-TLM-0078/20

This report only applies to the sample tested.  
This report shall not be reproduced other than in full except with the permission of the laboratory Testing reports without signature and seal are not valid

GTL-TLM-0078/20

12.11.2020

Test Report

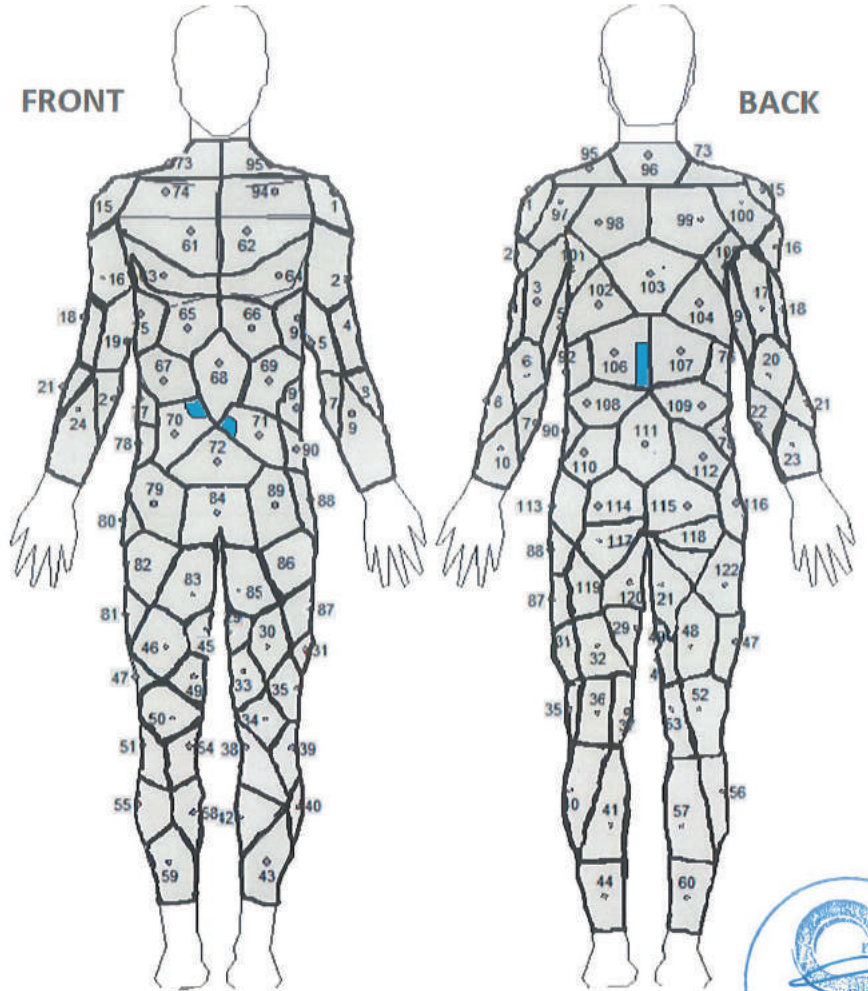


Figure 1 Region passing liquid



Report No: GTL-TLM-0078/20

This report only applies to the sample tested.  
This report shall not be reproduced other than in full except with the permission of the laboratory Testing reports without signature and seal are not valid

### ANALYSIS REPORT

Report No. : 2028323E Report Date : 16/11/2020  
 Applicant : UNIVERSAL SERTİFİKASYON VE GÖZETİM HİZ. TİC. LTD. ŞTİ  
 Address : Necip Fazıl Bulvarı Keyap Sitesi E2 Blok No:44/84- Yukarı Dudullu  
 Ümraniye/İstanbul/Turkey  
 Sample : Protective Coverall (S) Type: 5/6 / Category III / Amsterdam  
 Sample Package : Poly packing  
 Sample Amount : 5 pieces  
 Sampling Point : -  
 Sampling Date : 05/11/2020  
 Sample Lot No. : -  
 Production Date : 11/2020  
 Packing Date : -  
 Expire Date : 11/2025  
 Producer Company : Yalıtkan Paspas Kauçuk Ürünleri A.Ş.  
 Product No : -  
 Supplier Number : -  
 Sample Receiving Time : 06/11/2020 14:30:00  
 Analysis Beginning Time : 06/11/2020 14:45:00  
 Analysis Completion Time : 13/11/2020



Test TS EN ISO/IEC 17025 AB-0363-T
AB-0363-T
2028323E
11-20



Parameters	Unit	Finding	Method	Information
<b>Sentetik Kanın Nüfuzuna Karşı Direnç</b>				
The Average Thickness of the Material Tested	mm	0,236	ISO 16603	(*) 148
The Average Mass of the Material Tested	g	0,3666	ISO 16603	(*) 148
Test Spicemen 1: 0 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 1: 1,75 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 1: 3,5 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 1: 7 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 1: 14 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 1: 20 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen Thickness 1	mm	0,24	ISO 16603	(*)
Test Specimen Mass 1	g	0,3864	ISO 16603	(*)
Test Spicemen 2: 0 kPa	-	Succeed	ISO 16603	(*) 149

### ANALYSIS REPORT

Report No. : 2028323E Report Date : 16/11/2020



Test TS EN ISO/IEC 17025 AB-0363-T
AB-0363-T
2028323E
11-20

Parameters	Unit	Finding	Method	Information
Test Spicemen 2: 1,75 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 2: 3,5 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 2: 7 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 2: 14 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 2: 20 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen Thickness 2	mm	0,24	ISO 16603	(*)
Test Specimen Mass 2	g	0,3712	ISO 16603	(*)
Test Spicemen 3: 0 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 3: 1,75 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 3: 3,5 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 3: 7 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 3: 14 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen 3: 20 kPa	-	Succeed	ISO 16603	(*) 149
Test Spicemen Thickness 3	mm	0,23	ISO 16603	(*)
Test Specimen Mass 3	g	0,3424	ISO 16603	(*)
The Procedure Selected	-	D	ISO 16603	(*)
<b>Microbial Penetration - Dry Bacterium</b>				
Microbial Penetration - Dry Bacterium	log cfu	1,3	ISO 22612	(*) 150, 151
Test Spicemen 1 - Colony Count	cfu	32	-	(*)
Test Spicemen 2 - Colony Count	cfu	7	-	(*)
Test Spicemen 3 - Colony Count	cfu	19	-	(*)
Test Spicemen 4 - Colony Count	cfu	19	-	(*)
Test Spicemen 5 - Colony Count	cfu	16	-	(*)
Test Spicemen 6 - Colony Count	cfu	8	-	(*)
Test Spicemen 7 - Colony Count	cfu	15	-	(*)
Test Spicemen 8 - Colony Count	cfu	28	-	(*)
Test Spicemen 9 - Colony Count	cfu	16	-	(*)
Test Spicemen 10 - Colony Count	cfu	22	-	(*)



**Kübra HANCI AKAN**  
Microbiology Laboratory Responsible



Approved by  
17/11/2020  
**Ömer Yasin BALIK**  
Laboratory Manager



**Kübra HANCI AKAN**  
Microbiology Laboratory Responsible



Approved by  
17/11/2020  
**Ömer Yasin BALIK**  
Laboratory Manager

**ANALYSIS REPORT**

Report No. : 2028323E

Report Date : 16/11/2020



**ANALYSIS REPORT**

Report No. : 2028323E

Report Date : 16/11/2020



Parameters	Unit	Finding	Method	Information
Ortalama Koloni Sayısı	cfu	18	-	(*)
Negative Control Count 1	cfu	<1	-	(*)
Negative Control Count 2	cfu	<1	-	(*)
Talc Concentration	cfu/g	4*10 <sup>8</sup>	ISO 22612	(*)
<b>Microbial Penetration - Wet Bacterium</b>				
Test Spicemen 1 - Colony Count	cfu	231	ISO 22610	(*) 154
Test Spicemen 2 - Colony Count	cfu	200	ISO 22610	(*) 154
Test Spicemen 3 - Colony Count	cfu	212	ISO 22610	(*) 154
Test Spicemen 4 - Colony Count	cfu	122	ISO 22610	(*) 154
Test Spicemen 5 - Colony Count	cfu	169	ISO 22610	(*) 154
Test Spicemen 1 - Barrier Index	-	4,55	ISO 22610	(*) 154
Test Spicemen 2 - Barrier Index	-	4,52	ISO 22610	(*) 154
Test Spicemen 3 - Barrier Index	-	4,65	ISO 22610	(*) 154
Test Spicemen 4 - Barrier Index	-	5,03	ISO 22610	(*) 154
Test Spicemen 5 - Barrier Index	-	4,74	ISO 22610	(*) 154
Test Spicemen 1 - Percentage of Penetration	%	3,35	ISO 22610	(*) 154
Test Spicemen 2 - Percentage of Penetration	%	2,9	ISO 22610	(*) 154
Test Spicemen 3 - Percentage of Penetration	%	3,07	ISO 22610	(*) 154
Test Spicemen 4 - Percentage of Penetration	%	1,77	ISO 22610	(*) 154
Test Spicemen 5 - Percentage of Penetration	%	2,45	ISO 22610	(*) 154
Average Penetration Percentage	%	2,71	ISO 22610	(*)
Bacillus atrophæus Concentration	spores/mL	6,9*10 <sup>3</sup>	ISO 22610	(*)
<b>Pathogen Penetration</b>				
The Procedure Selected	-	D	ISO 16604	(*) 155
Hydrostatic Pressure - 1	kPa	20	ISO 16604	(*)
Test Spicemen 1	-	Succeed	ISO 16604	(*) 157
Hydrostatic Pressure - 2	kPa	20	ISO 16604	(*)
Test Spicemen 2	-	Succeed	ISO 16604	(*) 157



**Kübra HANCI AKAN**  
Microbiology Laboratory Responsible



Approved by  
17/11/2020  
**Ömer Yasin BALIK**  
Laboratory Manager



**Kübra HANCI AKAN**  
Microbiology Laboratory Responsible



Approved by  
17/11/2020  
**Ömer Yasin BALIK**  
Laboratory Manager

Parameters	Unit	Finding	Method	Information
Hydrostatic Pressure - 3	kPa	20	ISO 16604	(*)
Test Spicemen 3	-	Succeed	ISO 16604	(*) 157
Pre-test Bacteriophage Titer	pfu/mL	5,1*10 <sup>8</sup>	ISO 16604	(*)
Post-test Bacteriophage Titer	pfu/mL	3,6*10 <sup>8</sup>	ISO 16604	(*)
Negative Control	-	Succeed	ISO 16604	(*)
Positive Control	-	Fail	ISO 16604	(*)
<b>Source of Limit Ranges : 104 El ve Kol Koruması ve Can Yeleşü Dahil Korumucu Kıyafetler (EN 14126)</b>				
<b>Method</b>	ISO : International Organization for Standardization			
<b>Information</b>	<p>148 : Test sample-1 is sampled from the right arm, test sample-2 left leg, test sample-3 body part. The thickness and mass given are the average of the results for these three samples.</p> <p>149 : The retaining screen has 50% open area</p> <p>150 : Test Conditions : 65±5 relative humidity and 20±2°C ATCC 9372 Bacillus subtilis spores were used in the concentration of ethyl alcohol. 200 mm x 200 mm 12 test pieces used The vibrator was operated in an air flow with a vibration frequency of 20800 per minute. □ □</p> <p>151 : EN 14126 standard provides Class 2 values according to Table 4.</p> <p>154 : Test Conditions : 65±5 relative humidity and 20±2°C minimum 24 hours The distance to the distance agar-to-brim is 3.0 mm. 25 cm x 25 cm 5 test pieces were used. The tests were carried out from the outside of the sample. ATCC 9372 Bacillus atrophæus spore suspension was used. Incubator Control &lt;4 cfu Test Environment Control &lt;25 cfu □</p> <p>155 : Test Conditions: Minimum 24 hours at 20±2°C and 65±5 % relative humidity Sample size and number: 3 test samples in size 75x75mm Name of test microorganism: ATCC 13706-B1 Escherichia coli bacteriophage Phi X174 PFU: Plate forming unit</p> <p>157 : Test sample-1 right arm, test sample-2 left leg, test sample-3 were sampled from the body part.</p>			
<b>Note</b>	<p>1. When request, the conformit assessment is carried out in accordance with the legal regulations and standards or the decision rules which are agreed with the customer.</p> <p>2. Descriptive information about the samples / sampling in the analysis report has been declared by the customer. Our laboratory is not responsible for the legal losses.</p> <p>3. Analysis report covers samples/sampling that comes to the laboratory.</p> <p>4. This report and results don't be copied and printed partially or completely without permission of Cevre Industrial Analysis Laboratory for any commercial and advertising purposes.</p> <p>5. This report shall not be used official purposes related to Environmental Regulations.</p> <p>6. The test report without sign is not valid.</p> <p>7. (*) This parameter is covered by our accreditation scope.</p>			
End of Report				

Microbial Penetration - Wet Bacteria Analysis Report Attachment (ISO 22610)										
Sample No:		2028323E								
Analysis Results										
	Bacillus atrophaeus Spore Concentration (spore/mL)	X1 (cfu)	X2 (cfu)	X3 (cfu)	X4 (cfu)	X5 (cfu)	Z (cfu)	Total Colony Count (cfu)	% Pn	
		0-15 minute	15-30 minute	30-45 minute	45-60 minute	60-75 minute				
Test Specimen - 1	6900	13	16	54	51	97	106	231	3,35	
Test Specimen - 2		17	23	33	35	92	95	200	2,90	
Test Specimen - 3		10	24	41	57	80	130	212	3,07	
Test Specimen - 4		5	21	14	34	48	147	122	1,77	
Test Specimen - 5		9	28	17	40	75	110	169	2,45	
X1: 1.plates colony count										
X2: 2.plates colony count										
X3: 3.plates colony count										
X4: 4.plates colony count										
X5: 5.plates colony count										
Z: Number of plates in the reverse test sample										
Pn: Percentage of penetration										
Total Colony Count = X1+X2+X3+X4+X5										
	T (cfu)	CUM1	CUM2	CUM3	CUM4	CUM5	Barrier Index (EPP)	Donor (cfu)	Incubator Control (cfu)	Ambient Test Control (cfu)
Test Specimen - 1	337	0,04	0,09	0,25	0,40	0,69	4,55	155	<4	<25
Test Specimen - 2	295	0,06	0,14	0,25	0,37	0,68	4,52	112	<4	<25
Test Specimen - 3	342	0,03	0,10	0,22	0,39	0,62	4,65	127	<4	<25
Test Specimen - 4	269	0,02	0,10	0,15	0,28	0,45	5,01	169	<4	<25
Test Specimen - 5	279	0,03	0,13	0,19	0,34	0,61	4,70	121	<4	<25
T = Z + X1 + X2 + X3 + X4 + X5										
CUM1 = X1/T										
CUM2 = (X2 + X1)/T										
CUM3 = (X3 + X2 + X1)/T										
CUM4 = (X4 + X3 + X2 + X1)/T										
CUM5 = (X5 + X4 + X3 + X2 + X1)/T										



*Global export from Turkey to 4 continents and 17 countries...*



Ömer Yasin BALIK  
Laboratory Manager